

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050322\
 Data File : PD069409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2022 18:36
 Operator : AR\AJ
 Sample : N2615-17
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 01:22:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	4.171	21905943	223.5E6	17.290	18.515
2)	SA Decachlor...	8.197	9.364	34073442	201.5E6	25.623	28.655
Target Compounds							
3)	MA gamma-BHC...	4.167	0.000	1435296	0	0.794	N.D. #
4)	MA Heptachlor	0.000	5.366	0	4101490	N.D.	0.271
5)	MB Aldrin	0.000	5.653f	0	511922	N.D.	<MDL
7)	B delta-BHC	0.000	5.221f	0	3862534	N.D.	0.329
8)	B Heptachlo...	0.000	6.101	0	742132	N.D.	<MDL
9)	A Endosulfan I	0.000	6.454	0	482553	N.D.	<MDL
10)	B trans-Chl...	0.000	6.380f	0	738986	N.D.	<MDL
11)	B cis-Chlor...	0.000	6.380	0	738986	N.D.	<MDL
12)	B 4,4'-DDE	0.000	6.614f	0	805669	N.D.	<MDL
14)	MA Endrin	0.000	6.880f	0	26086	N.D.	<MDL
15)	B Endosulfa...	0.000	7.101	0	2067302	N.D.	0.216
16)	A 4,4'-DDD	0.000	6.991f	0	346880	N.D.	<MDL
17)	MA 4,4'-DDT	6.366	0.000	379255	0	0.309	N.D. #
20)	A Methoxychlor	0.000	7.813	0	1405425	N.D.	0.341
22)	Toxaphene-1	0.000	6.614	0	805669	N.D.	17.079
24)	Toxaphene-3	6.366f	0.000	379255	0	16.002	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050322\
Data File : PD069409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2022 18:36
Operator : AR\AJ
Sample : N2615-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 01:22:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

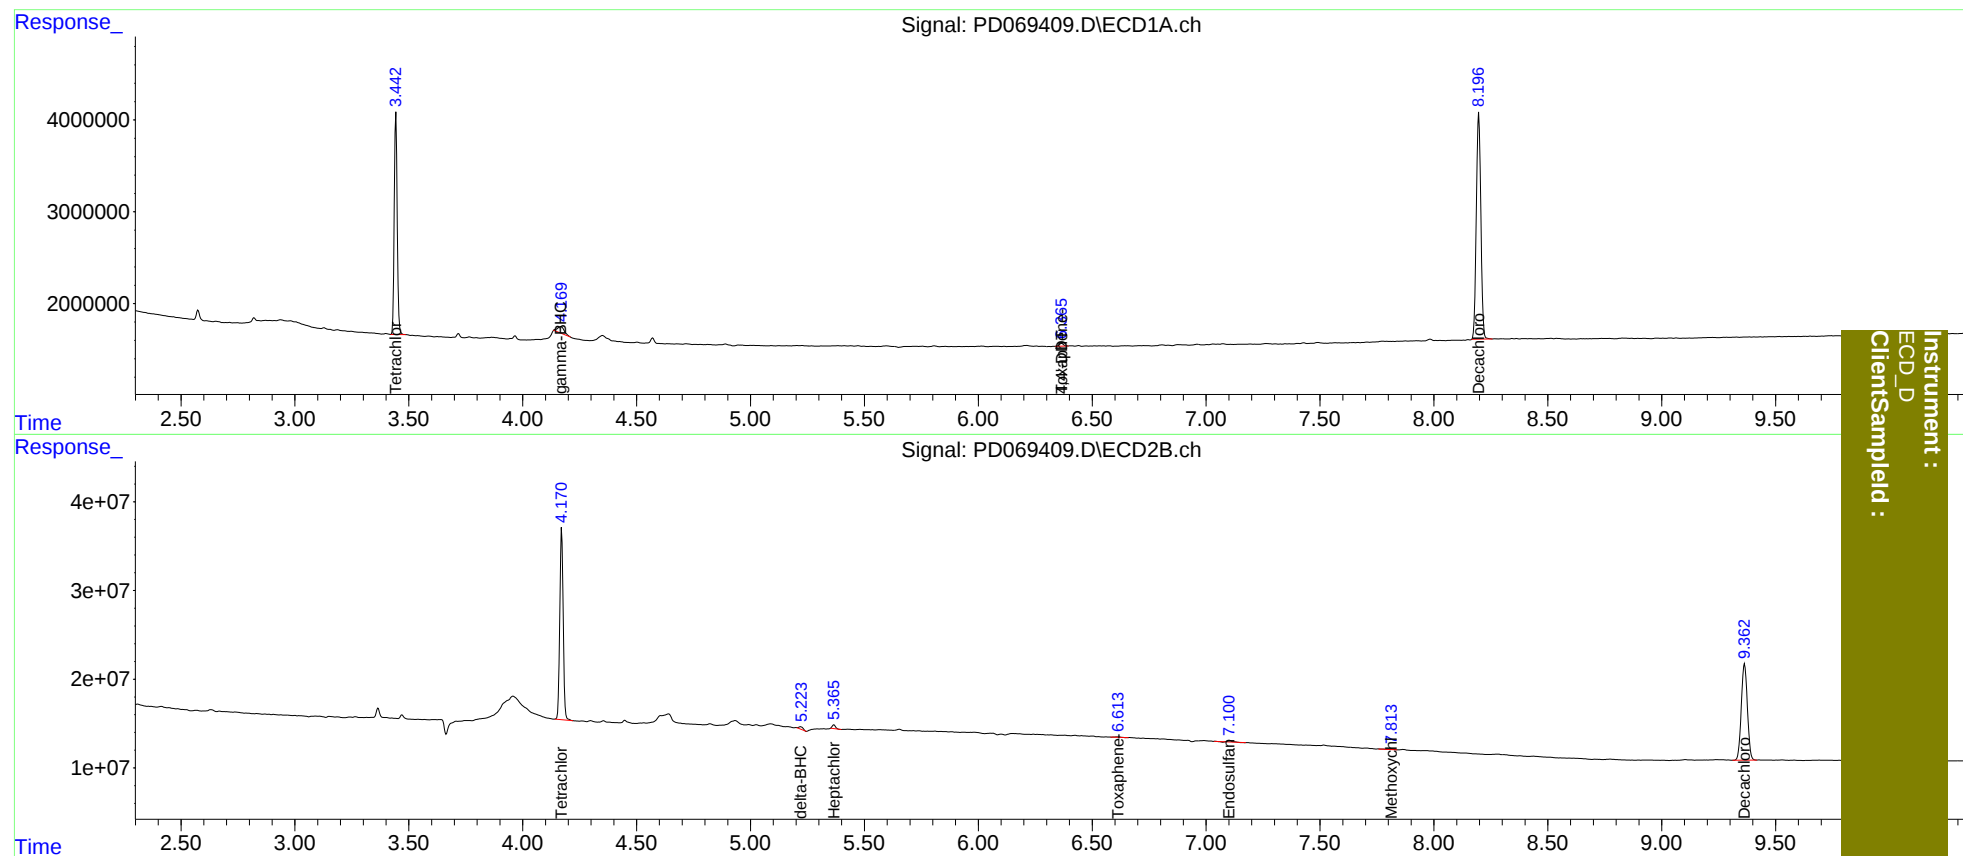


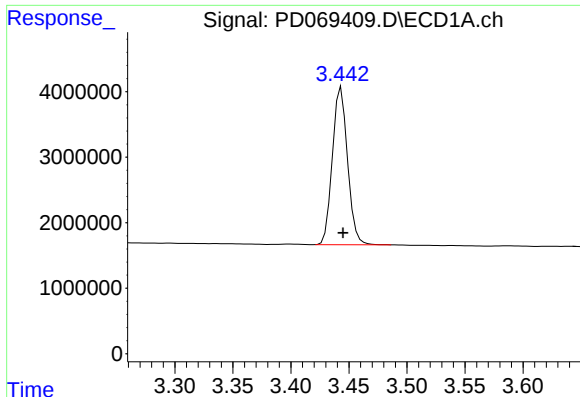

#1 Tetrachloro-m-xylene


R.T.: 3.443 min
Delta R.T.: -0.002 min
Response: 21905943
Conc: 17.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

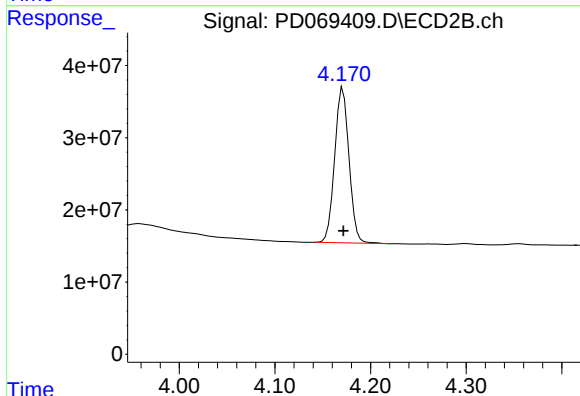


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 223460318
Conc: 18.51 ng/ml

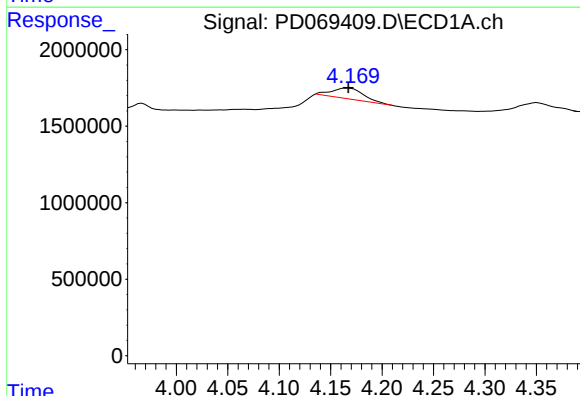


#3 gamma-BHC (Lindane)

R.T.: 4.167 min
Delta R.T.: 0.000 min
Response: 1435296
Conc: 0.79 ng/ml

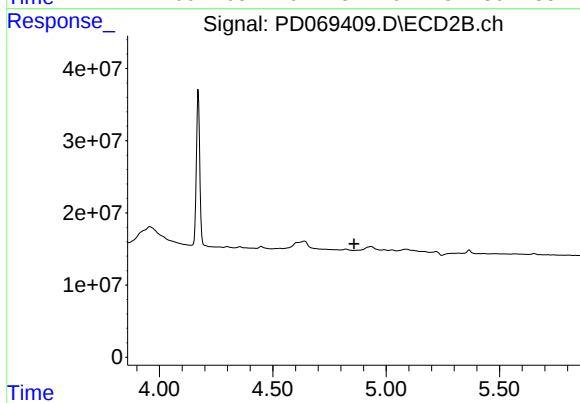

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.859 min
Response: 0
Conc: N.D.

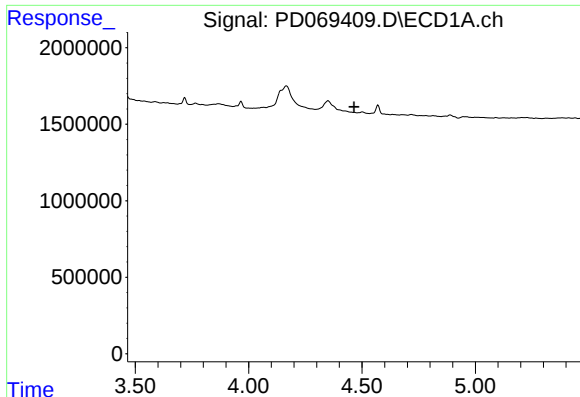

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

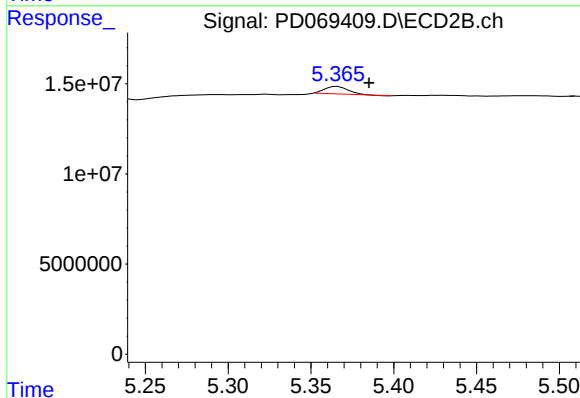


#4 Heptachlor

R.T.: 5.366 min
Delta R.T.: -0.019 min
Response: 4101490
Conc: 0.27 ng/ml

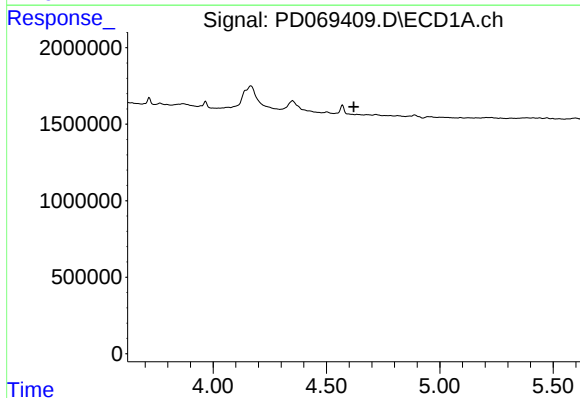


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.621 min
Response: 0
Conc: N.D.

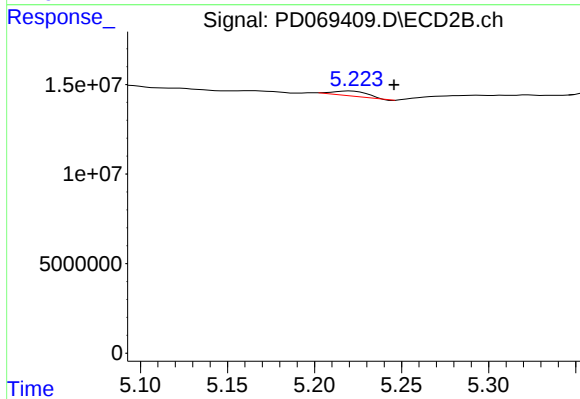

#7 delta-BHC


R.T.: 5.221 min
Delta R.T.: -0.025 min
Response: 3862534
Conc: 0.33 ng/ml

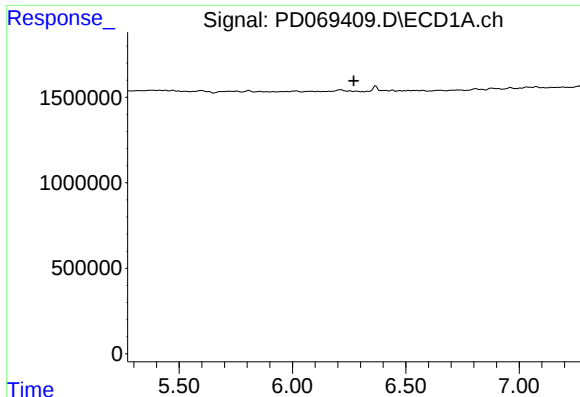

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

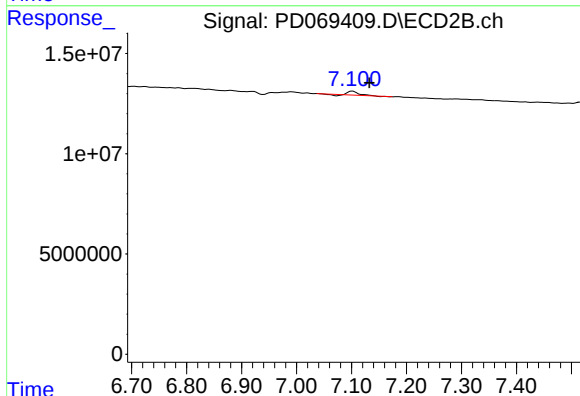


#15 Endosulfan II

R.T.: 7.101 min
Delta R.T.: -0.031 min
Response: 2067302
Conc: 0.22 ng/ml

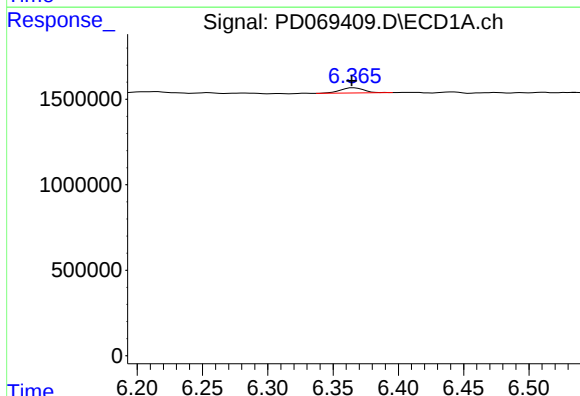


#17 4,4'-DDT

R.T.: 6.366 min
Delta R.T.: 0.002 min
Response: 379255
Conc: 0.31 ng/ml

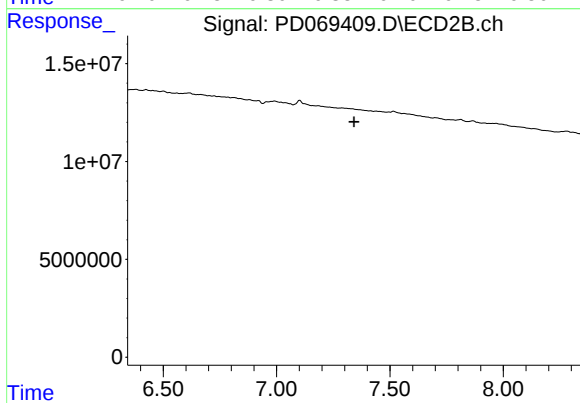

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.

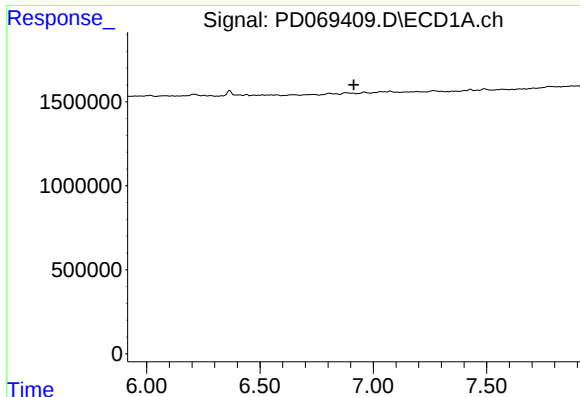

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

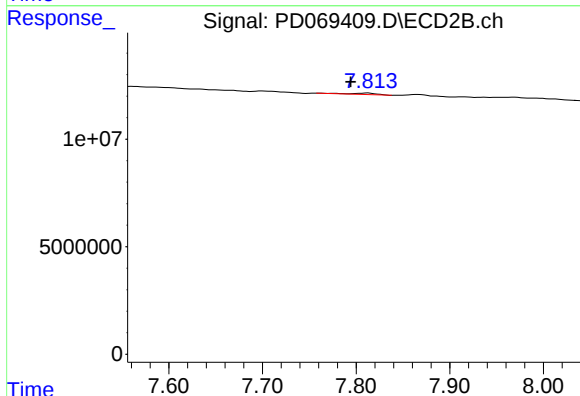


#20 Methoxychlor

R.T.: 7.813 min
Delta R.T.: 0.018 min
Response: 1405425
Conc: 0.34 ng/ml

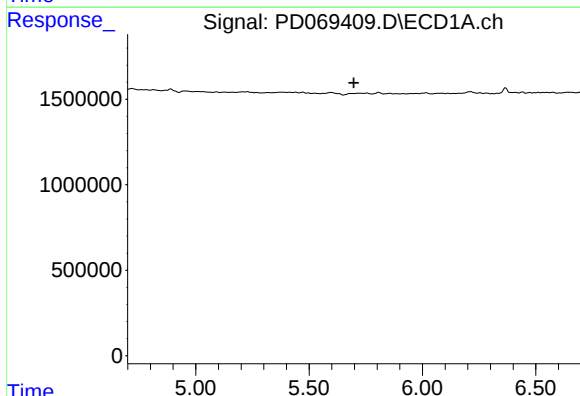


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.697 min
Response: 0
Conc: N.D.

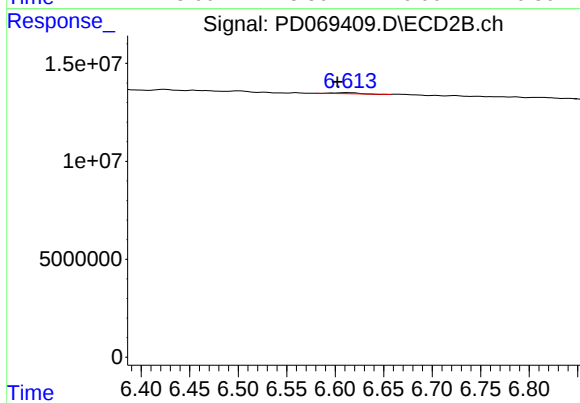

#22 Toxaphene-1


R.T.: 6.614 min
Delta R.T.: 0.012 min
Response: 805669
Conc: 17.08 ng/ml

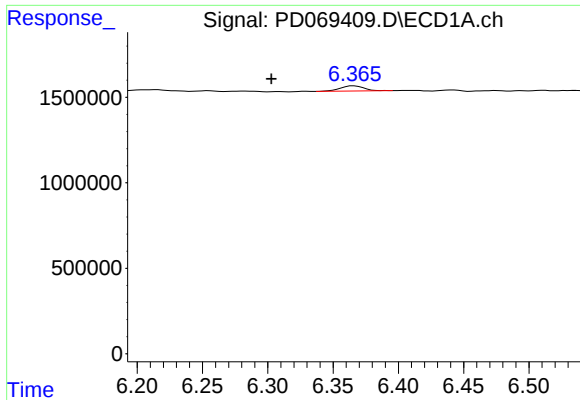

#24 Toxaphene-3


R.T.: 6.366 min
Delta R.T.: 0.063 min
Response: 379255
Conc: 16.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

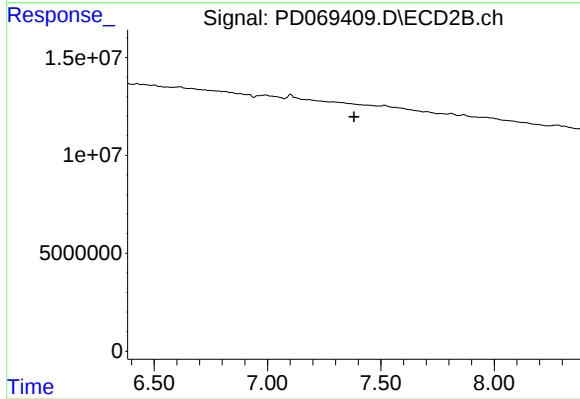


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 7.382 min
Response: 0
Conc: N.D.

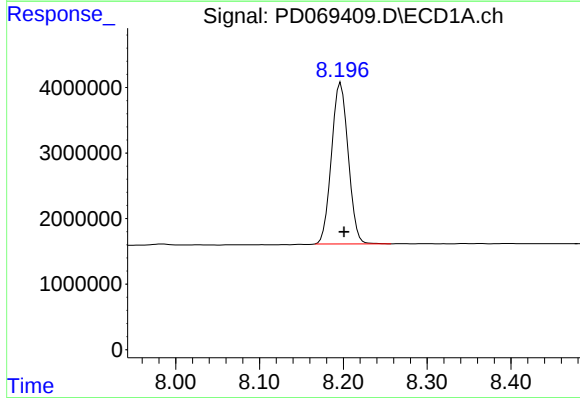

#27 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.004 min
Response: 34073442
Conc: 25.62 ng/ml

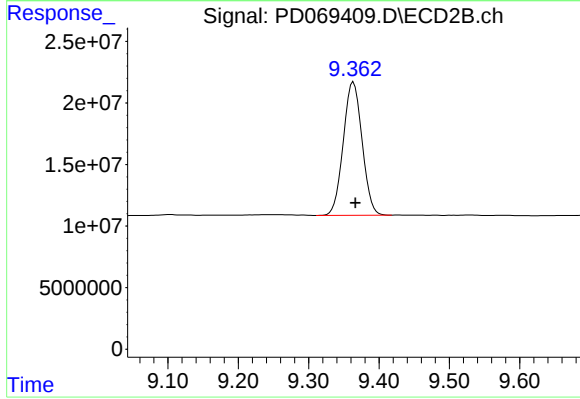

#27 Decachlorobiphenyl

R.T.: 9.364 min
Delta R.T.: -0.003 min
Response: 201503203
Conc: 28.65 ng/ml