

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050322\
 Data File : PD069385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2022 10:49
 Operator : AR\AJ
 Sample : N2615-06MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH0D2MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 01:09:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	20022605	201.1E6	15.804	16.664
2)	SA Decachlor...	8.196	9.364	29693784	151.1E6	22.330	21.482
Target Compounds							
2)	A alpha-BHC	3.883	4.567	85197750	685.9E6	47.664	41.724
3)	MA gamma-BHC...	4.165	4.857	83199887	658.1E6	45.997	42.237
4)	MA Heptachlor	4.463	5.384	77881080	627.8E6	45.871	41.468
5)	MB Aldrin	4.710	5.697	76749694	601.3E6	48.180	42.125
6)	B beta-BHC	4.416	5.020	36318016	284.3E6	46.888	42.379
7)	B delta-BHC	4.620	5.246	35784152	264.4E6	22.418	22.527
8)	B Heptachlo...	5.154	6.085	74375636	532.0E6	50.525	47.750
9)	A Endosulfan I	5.492	6.447	69355719	506.7E6	47.528	42.662
10)	B trans-Chl...	5.379	6.321	74782045	545.5E6	49.882	42.995
11)	B cis-Chlor...	5.438	6.397	73153453	531.0E6	49.009	42.634
12)	B 4,4'-DDE	5.604	6.547	143.4E6	1000.1E6	106.908	91.926
13)	MA Dieldrin	5.736	6.706	157.9E6	1085.9E6	101.472	90.030
14)	MA Endrin	5.994	6.926	138.3E6	873.2E6	98.832	89.791
15)	B Endosulfa...	6.267	7.131	131.2E6	854.3E6	101.847	89.133
16)	A 4,4'-DDD	6.121	7.037	121.8E6	823.5E6	99.907	87.938
17)	MA 4,4'-DDT	6.361	7.340	118.4E6	787.7E6	96.556	87.508
18)	B Endrin al...	6.437	7.255	104.2E6	667.8E6	105.011	93.462
19)	B Endosulfa...	6.649	7.480	113.2E6	706.5E6	90.312	80.520
20)	A Methoxychlor	6.912	7.794	315.5E6	1778.0E6	464.814	431.436
21)	B Endrin ke...	7.142	7.955	152.2E6	851.6E6	105.343	92.245

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050322\
Data File : PD069385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2022 10:49
Operator : AR\AJ
Sample : N2615-06MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 01:09:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

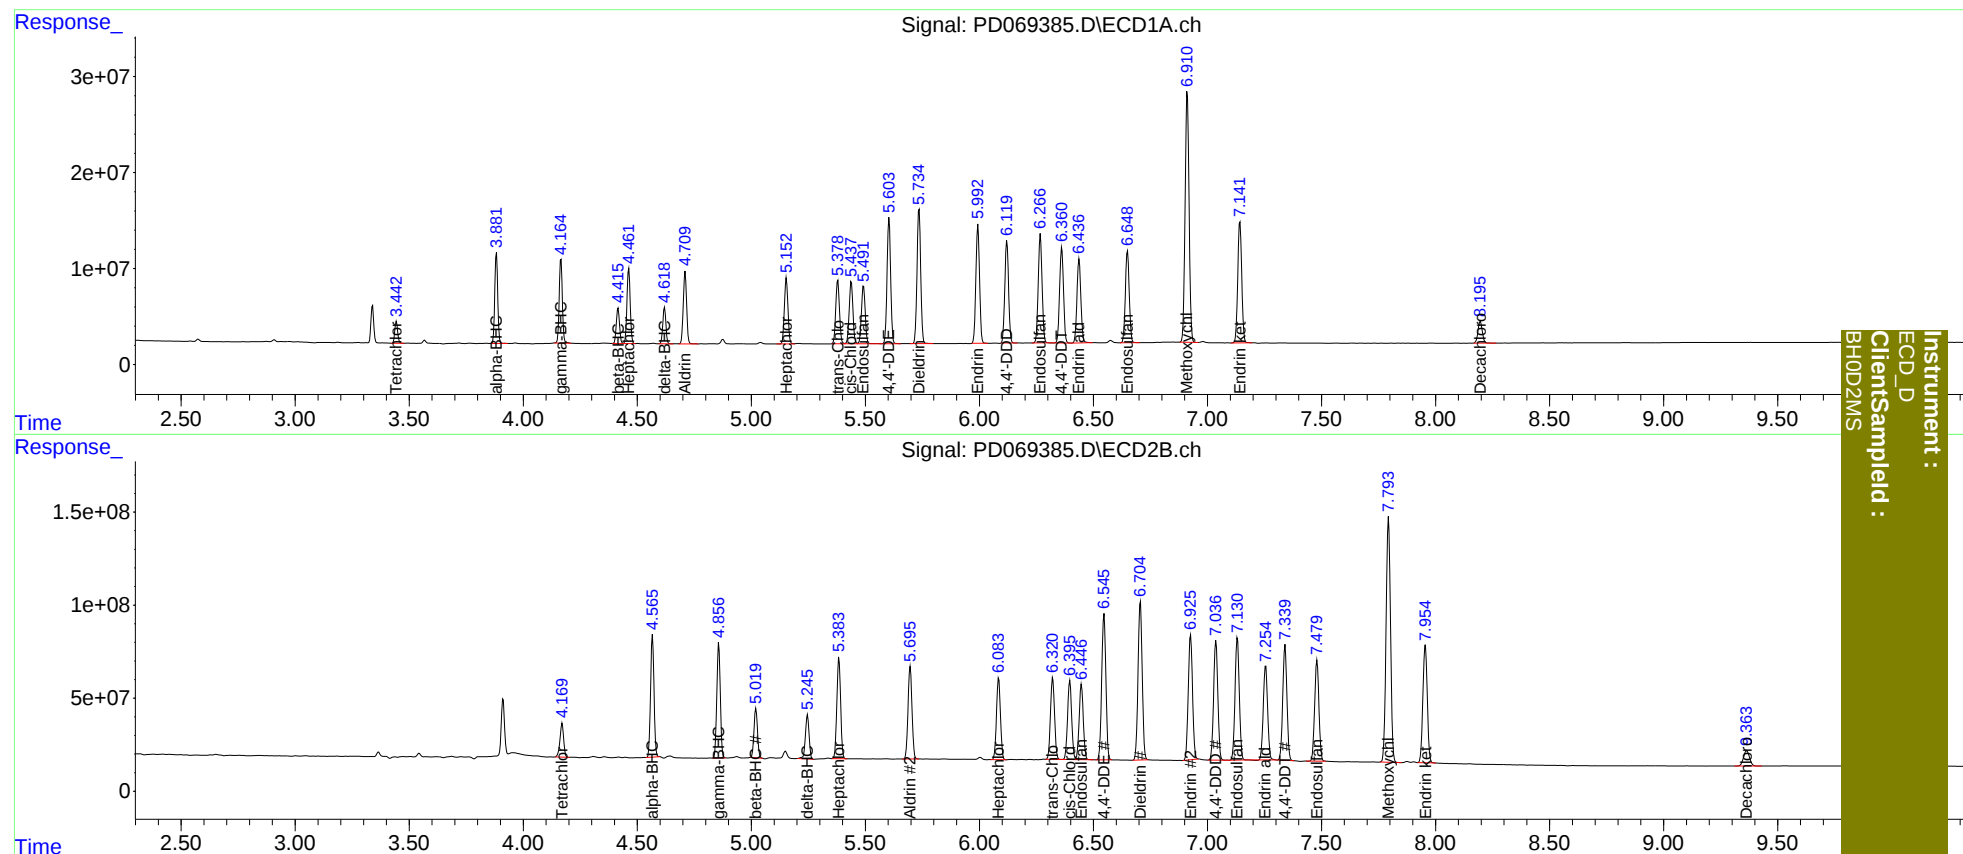

Instrument :
ECD_D
ClientSampled :
BH0D2MS