

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD050323\  
 Data File : PD075159.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 May 2023 15:14  
 Operator : AR\AJ  
 Sample : INDA501  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 03 15:26:58 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD050323CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Wed May 03 15:25:13 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
-----						
System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.771	178.9E6	81356389	78.233	76.940
27) SA Decachlor...	9.098	7.922	373.6E6	140.0E6	151.718	147.479
Target Compounds						
2) A alpha-BHC	4.006	3.274	333.7E6	131.0E6	86.555	83.992
3) MA gamma-BHC...	4.340	3.605	305.9E6	121.5E6	84.798	82.487
4) MA Heptachlor	4.932	3.946	312.7E6	119.0E6	83.796	80.797
9) A Endosulfan I	6.090	5.100	245.2E6	95530045	81.436	79.230
13) MA Dieldrin	6.366	5.366	581.2E6	225.2E6	169.164	164.085
14) MA Endrin	6.597	5.641	490.4E6	197.5E6	167.579	161.443
16) A 4,4'-DDD	6.730	5.789	418.7E6	165.1E6	168.515	163.781
17) MA 4,4'-DDT	7.045	6.041	448.7E6	175.9E6	175.245	170.841
20) A Methoxychlor	7.521	6.617	1196.5E6	428.7E6	801.458	730.692
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD050323\  
 Data File : PD075159.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 May 2023 15:14  
 Operator : AR\AJ  
 Sample : INDA501  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 03 15:26:58 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD050323CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Wed May 03 15:25:13 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

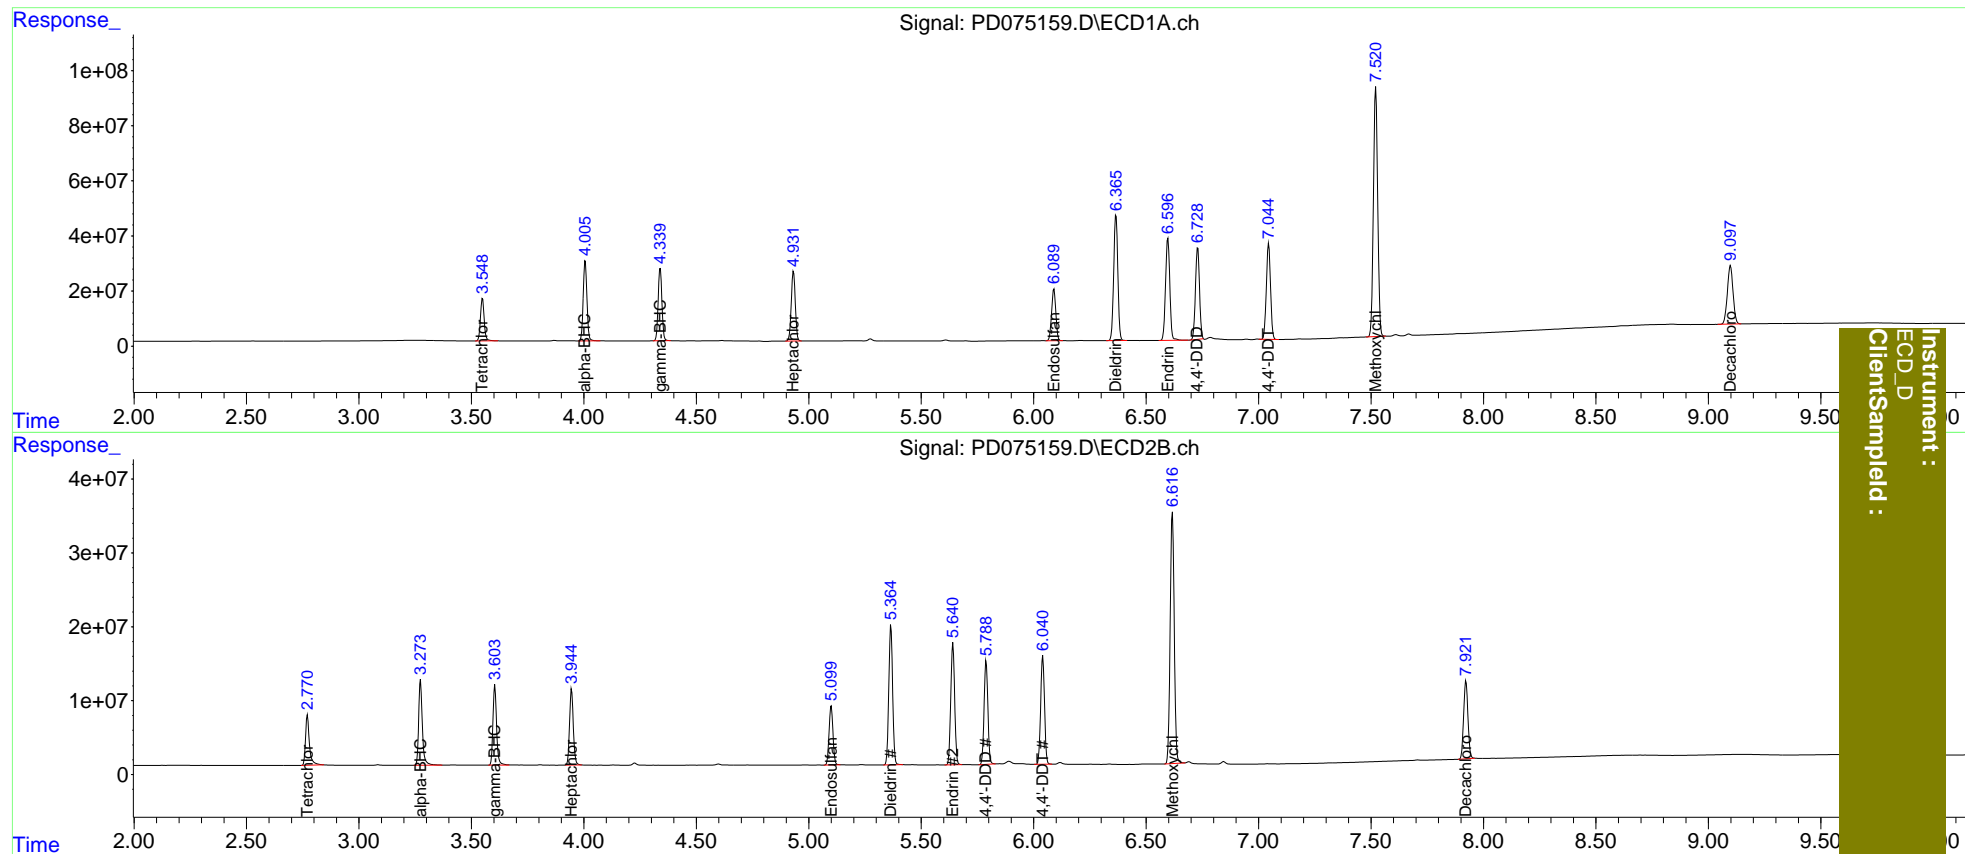

Instrument :  
 ECD\_D  
 ClientSampled :