

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
 Data File : PD075198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 05:51
 Operator : AR\AJ
 Sample : 02447-16
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 09:12:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.771	66949544	13815166	29.353	13.098 #
27)	SA Decachlor...	9.093	7.917	102.5E6	42673376	41.402	45.186
Target Compounds							
2)	A alpha-BHC	3.999	3.275	-6870107	7727293	N.D.	4.989
3)	MA gamma-BHC...	4.345	3.616	224.1E6	27874849	62.321	18.963 #
4)	MA Heptachlor	4.887f	3.959	539.7E6	3895.1E6	144.772	2665.702 #
5)	MB Aldrin	5.301f	4.241	2918.3E6	1257.7E6	800.062	848.029
6)	B beta-BHC	4.514	3.860f	1099.3E6	165.8E6	669.688	227.633 #
7)	B delta-BHC	4.824f	4.140	2346.2E6	1328.9E6	694.123	841.004
8)	B Heptachlo...	5.694	4.721	8847.2E6	70259886	2610.325	50.374 #
9)	A Endosulfan I	6.071	5.097	1002.0E6	2158428	332.194	1.798 #
10)	B trans-Chl...	5.978	4.956	4023.7E6	1785.8E6	1227.989	1308.700
11)	B cis-Chlor...	6.038	5.029	225.2E6	2009.7E6	66.087	1440.040 #
12)	B 4,4'-DDE	6.208	5.216	13075.6E6	-87389893	4004.075	N.D. #
13)	MA Dieldrin	6.361	5.365	1214.6E6	8772.1E6	355.177	6429.327 #
14)	MA Endrin	6.593	5.644	24424.0E6	1660.1E6	8445.966	1364.833 #
15)	B Endosulfa...	6.808	5.921	288.2E6	8247.6E6	89.488	6446.070 #
16)	A 4,4'-DDD	6.736	5.805	13030.3E6	-694277	5392.121	N.D. #
17)	MA 4,4'-DDT	7.019	6.034	17603.4E6	12889.4E6	6935.272	12788.713 #
18)	B Endrin al...	6.956	6.095	3788.7E6	605.8E6	1601.586	596.574 #
19)	B Endosulfa...	0.000	6.334	0	560.7E6	N.D.	482.061
20)	A Methoxychlor	7.507	6.590	113.1E6	851.9E6	76.970	1487.227 #
21)	B Endrin ke...	7.686	6.842	5690568	-970283	1.877	N.D. #
22)	Toxaphene-1	6.296	5.007	20558.9E6	3183.9E6	893632.215	460985.256 #
23)	Toxaphene-2	6.469	5.708	5478.9E6	5762.7E6	183616.288	721714.902 #
24)	Toxaphene-3	6.668	5.979	2305.7E6	2099.0E6	109305.773	239571.235 #
25)	Toxaphene-4	0.000	6.590	0	851.9E6	N.D.	33646.754

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
Data File : PD075198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 05:51
Operator : AR\AJ
Sample : 02447-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 09:12:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
Quant Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Signal #2 Phase: ZB-MR2

Signal: PD075198.D\ECD1A.ch

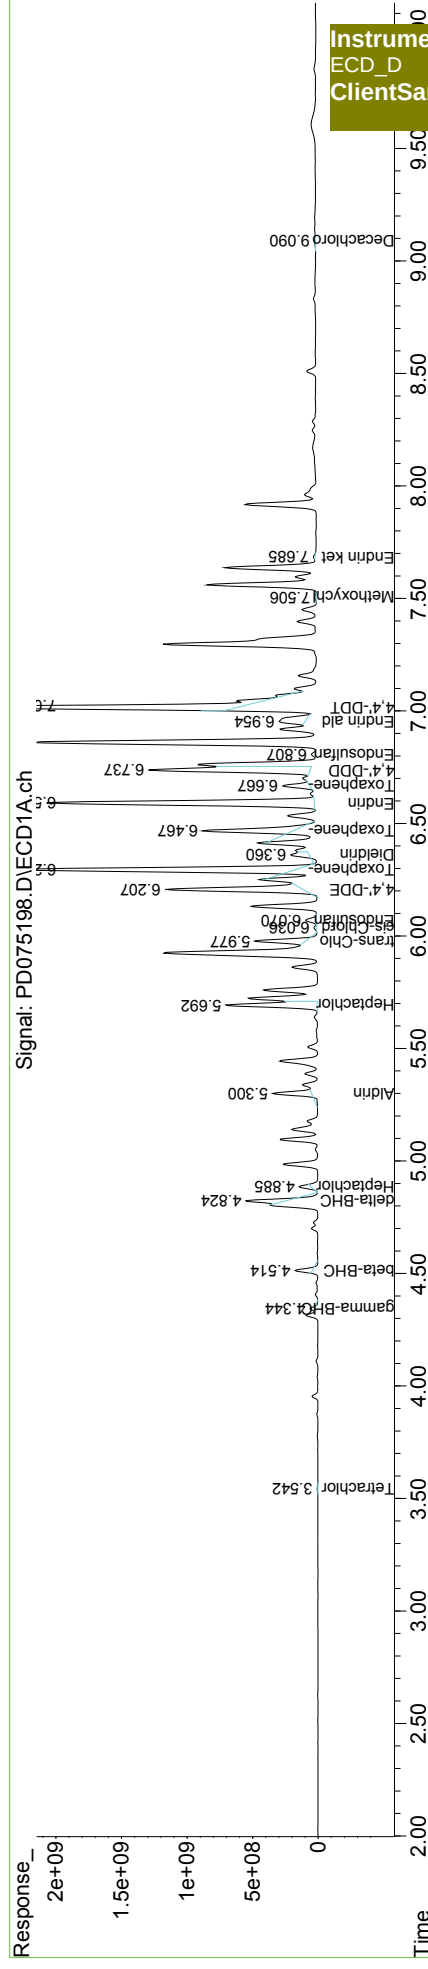

Signal: PD075198.D\ECD2B.ch

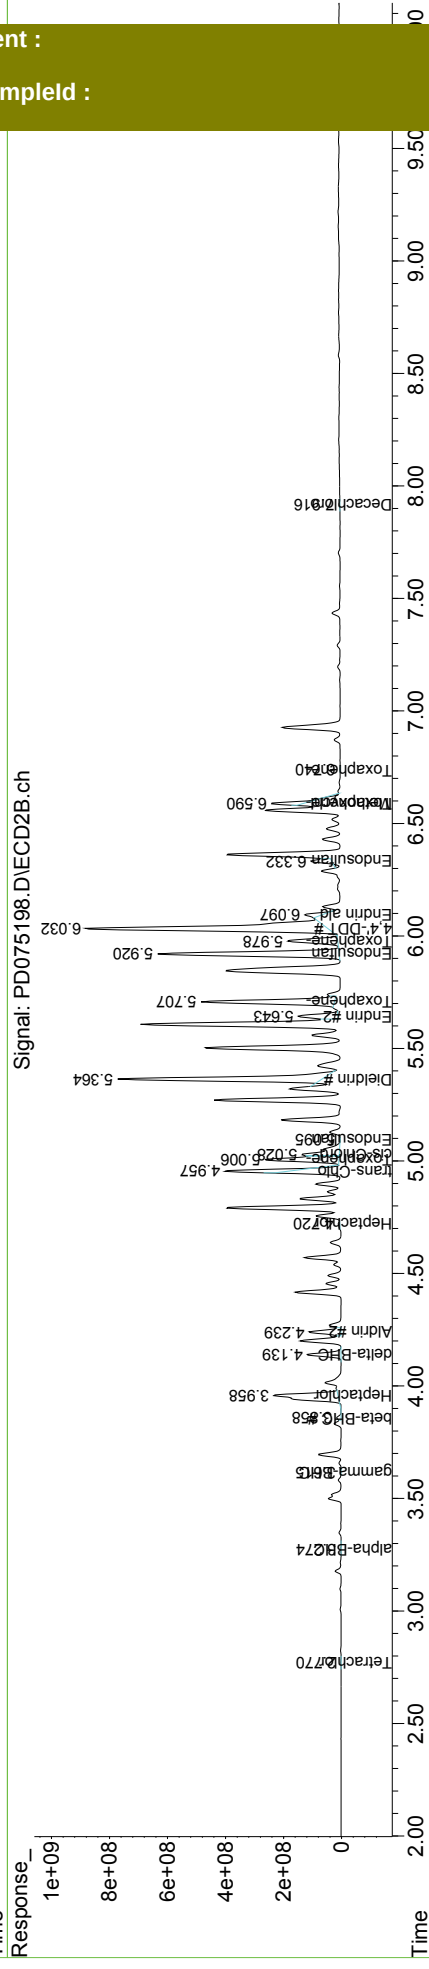

Instrument :
ECD_D
ClientSampleId :