

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
 Data File : PD075183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 22:51
 Operator : AR\AJ
 Sample : INDA405
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3209

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 02:41:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.771	46850231	21482504	20.541	20.368
27)	SA Decachlor...	9.094	7.920	102.9E6	40389709	41.586	42.768
Target Compounds							
2)	A alpha-BHC	4.005	3.273	78780335	31623637	20.486	20.416
3)	MA gamma-BHC...	4.338	3.603	74206623	30206637	20.641	20.550
4)	MA Heptachlor	4.930	3.944	77024450	30078552	20.661	20.585
9)	A Endosulfan I	6.088	5.098	61846742	24651953	20.503	20.541
13)	MA Dieldrin	6.364	5.364	141.4E6	56104378	41.337	41.121
14)	MA Endrin	6.595	5.639	120.1E6	50023940	41.547	41.127
16)	A 4,4'-DDD	6.727	5.787	105.1E6	42491442	43.472	42.861
17)	MA 4,4'-DDT	7.043	6.039	105.1E6	42784021	41.408	42.450
20)	A Methoxychlor	7.518	6.614	312.2E6	122.3E6	212.569	213.543

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
Data File : PD075183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2023 22:51
Operator : AR\AJ
Sample : INDA405
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 02:41:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

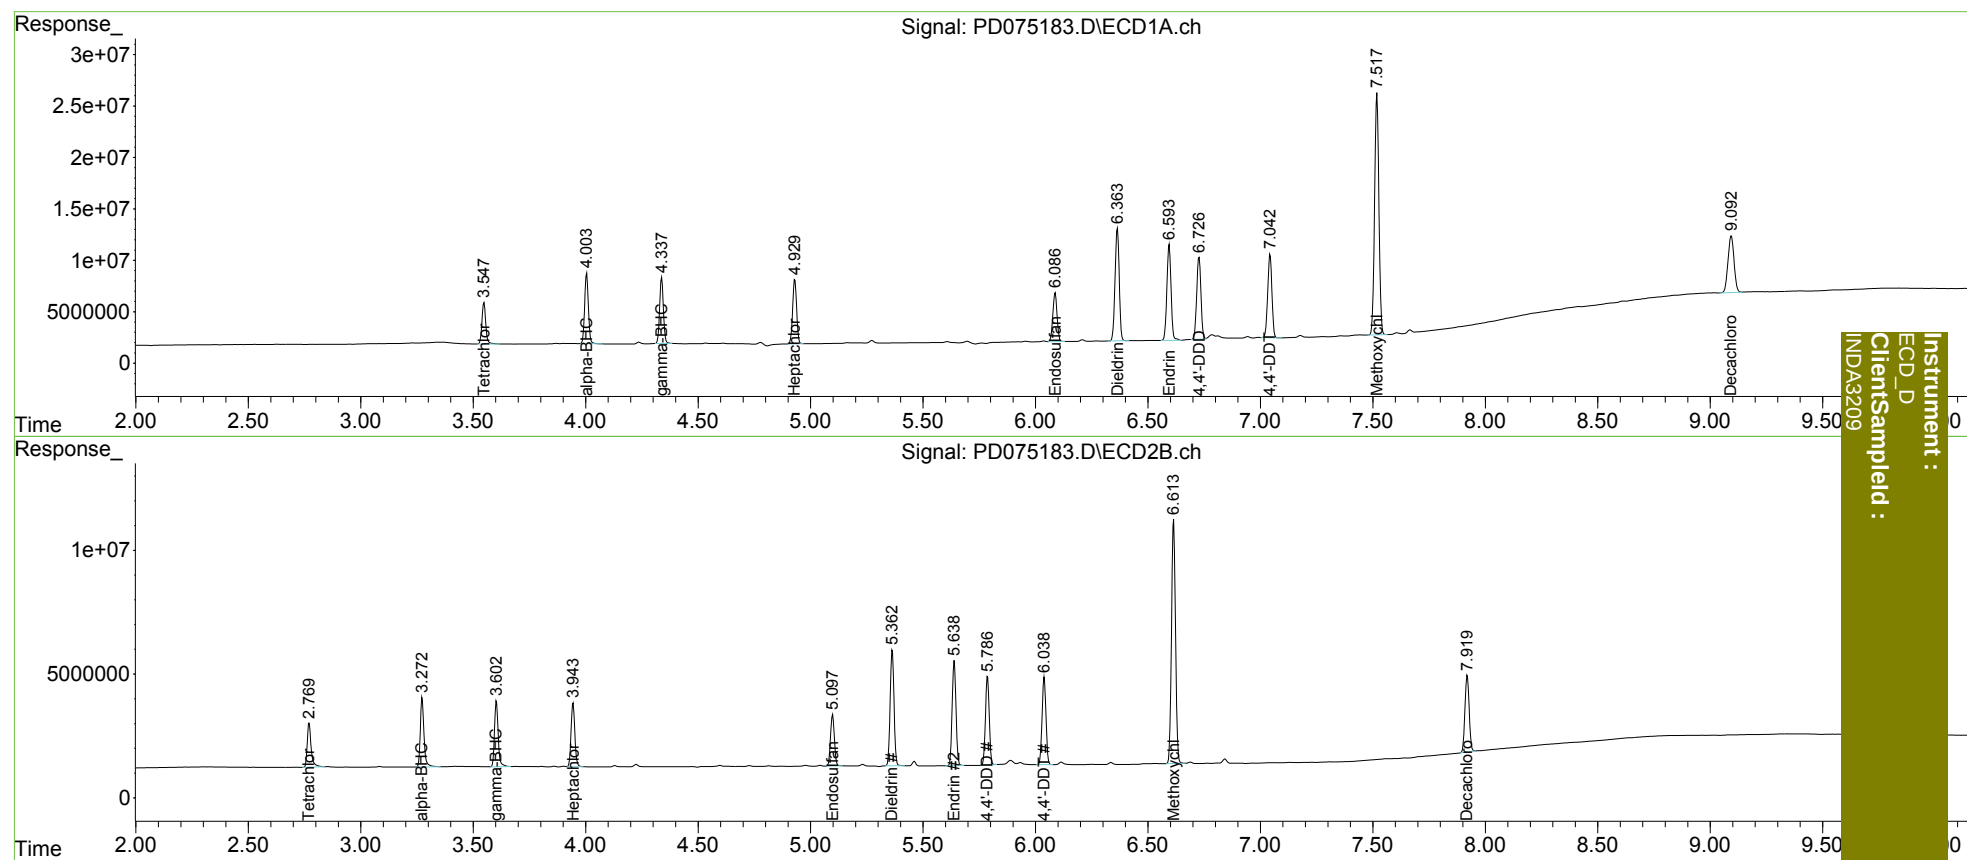

Instrument :
ECD_D
ClientSampled :
INDA3209