

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
 Data File : PD075166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 19:01
 Operator : AR\AJ
 Sample : 02419-34DL2 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW929DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/04/2023
 Supervised By : Ankita Jodhani 05/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 02:56:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	9.093	7.916	2892560	1212402	1.169m	1.284m
Target Compounds							
14)	MA Endrin	6.592	5.607	236.7E6	99428140	81.835	81.745m
17)	MA 4,4'-DDT	7.016	6.033	233.0E6	122.9E6	91.811m	121.920m#
19)	B Endosulfa...	7.159	6.333	19017891	8766876	6.914m	7.538m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
Data File : PD075166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2023 19:01
Operator : AR\AJ
Sample : 02419-34DL2 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 02:56:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

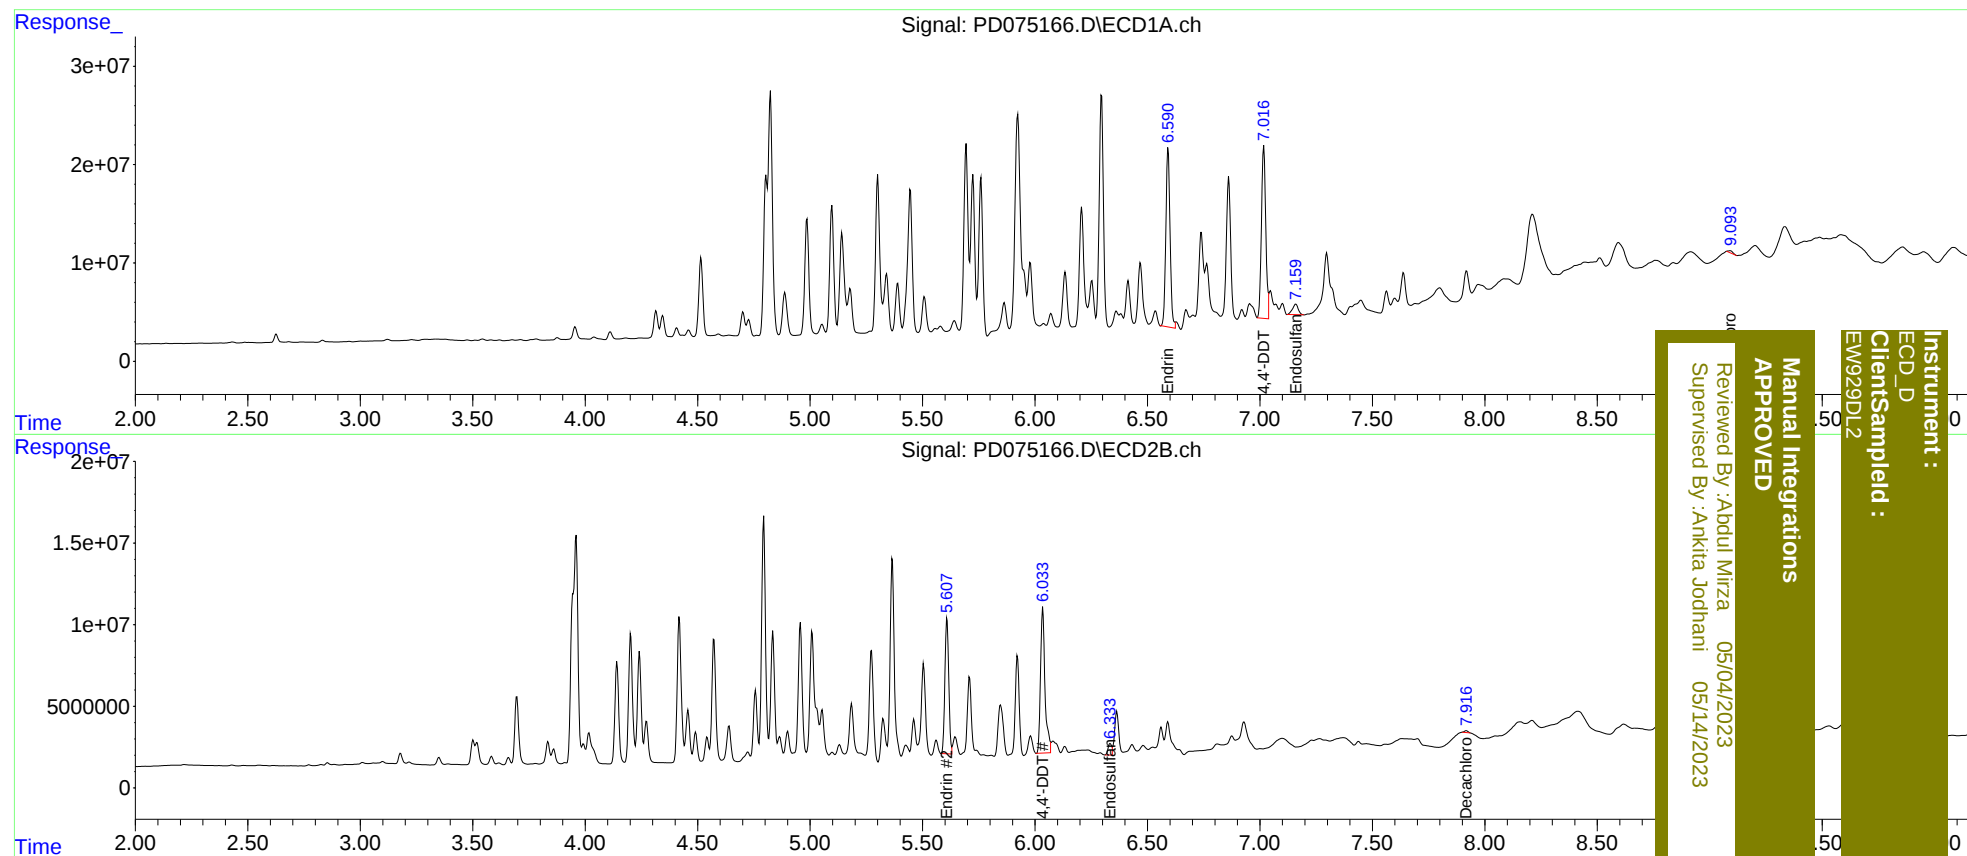

Instrument :
ECD_D
ClientSampled :
EW929DL2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/14/2023

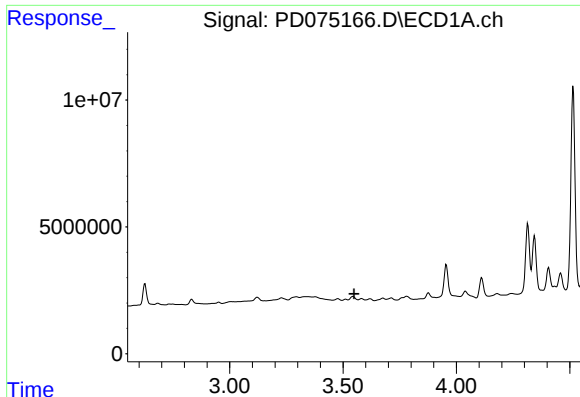


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EW929DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/14/2023

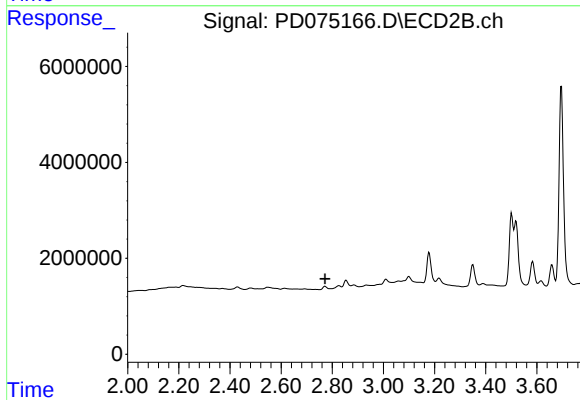


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.771 min
Response: 0
Conc: N.D.

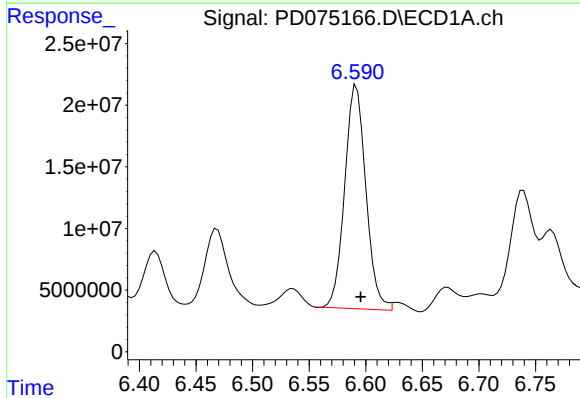


#14 Endrin

R.T.: 6.592 min
Delta R.T.: -0.003 min
Response: 236650803
Conc: 81.84 ng/ml

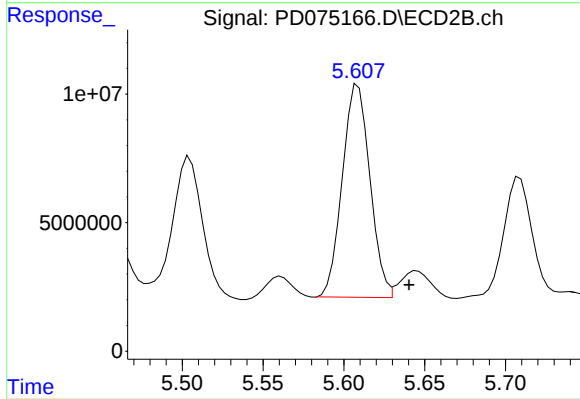

#14 Endrin

R.T.: 5.607 min
Delta R.T.: -0.033 min
Response: 99428140
Conc: 81.75 ng/ml m

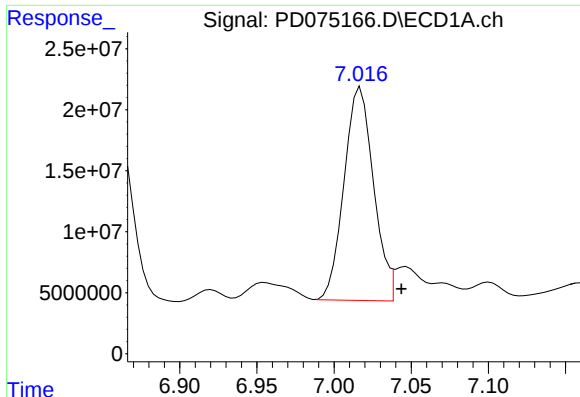


#17 4,4'-DDT

R.T.: 7.016 min
Delta R.T.: -0.028 min
Response: 233037856
Conc: 91.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW929DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/14/2023

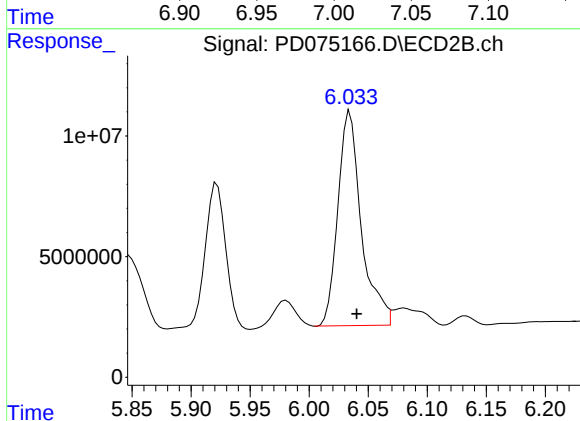


#17 4,4'-DDT

R.T.: 6.033 min
Delta R.T.: -0.007 min
Response: 122879899
Conc: 121.92 ng/ml m

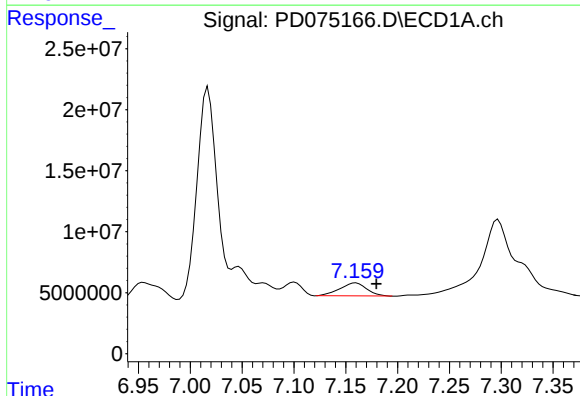


#19 Endosulfan Sulfate

R.T.: 7.159 min
Delta R.T.: -0.021 min
Response: 19017891
Conc: 6.91 ng/ml m

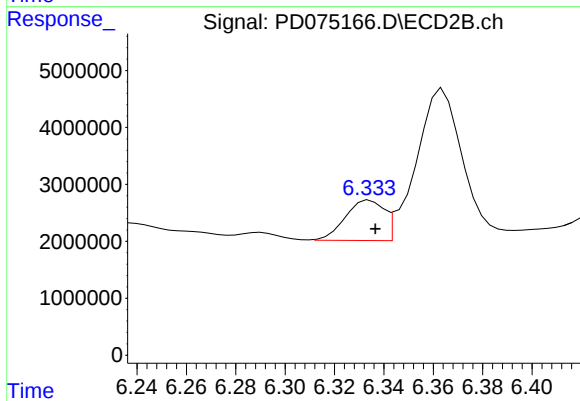

#19 Endosulfan Sulfate

R.T.: 6.333 min
Delta R.T.: -0.004 min
Response: 8766876
Conc: 7.54 ng/ml m

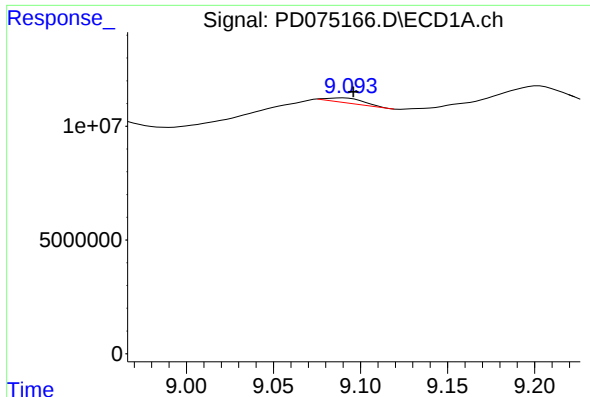


#27 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.003 min
Response: 2892560
Conc: 1.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW929DL2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/14/2023

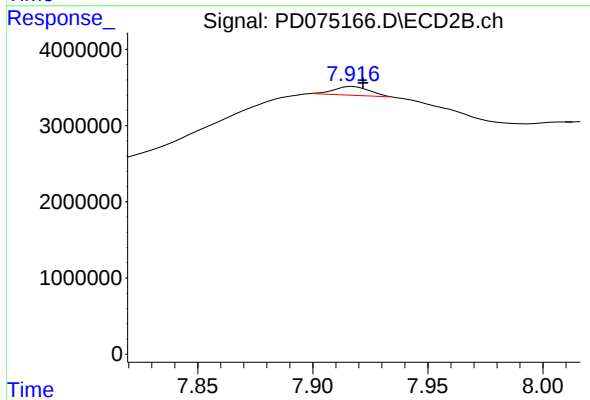

#27 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: -0.006 min
Response: 1212402
Conc: 1.28 ng/ml m