

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
 Data File : PD075167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 19:15
 Operator : AR\AJ
 Sample : 02419-35DL 4X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW930DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/04/2023
 Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 02:56:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.771	10352776	3841071	4.539	3.642
2)	SA Decachlor...	9.096	7.920	22963586	8244629	9.279m	8.730
Target Compounds							
3)	MA gamma-BHC...	4.343	3.612	29000668	2764175	8.067m	1.880 #
7)	B delta-BHC	4.802	4.141	109.5E6	42466254	32.383m	26.876
14)	MA Endrin	6.592	5.607	131.5E6	59131515	45.489	48.615m
17)	MA 4,4'-DDT	7.016	6.032	154.7E6	74540069	60.935m	73.958m


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
Data File : PD075167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2023 19:15
Operator : AR\AJ
Sample : 02419-35DL 4X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 02:56:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

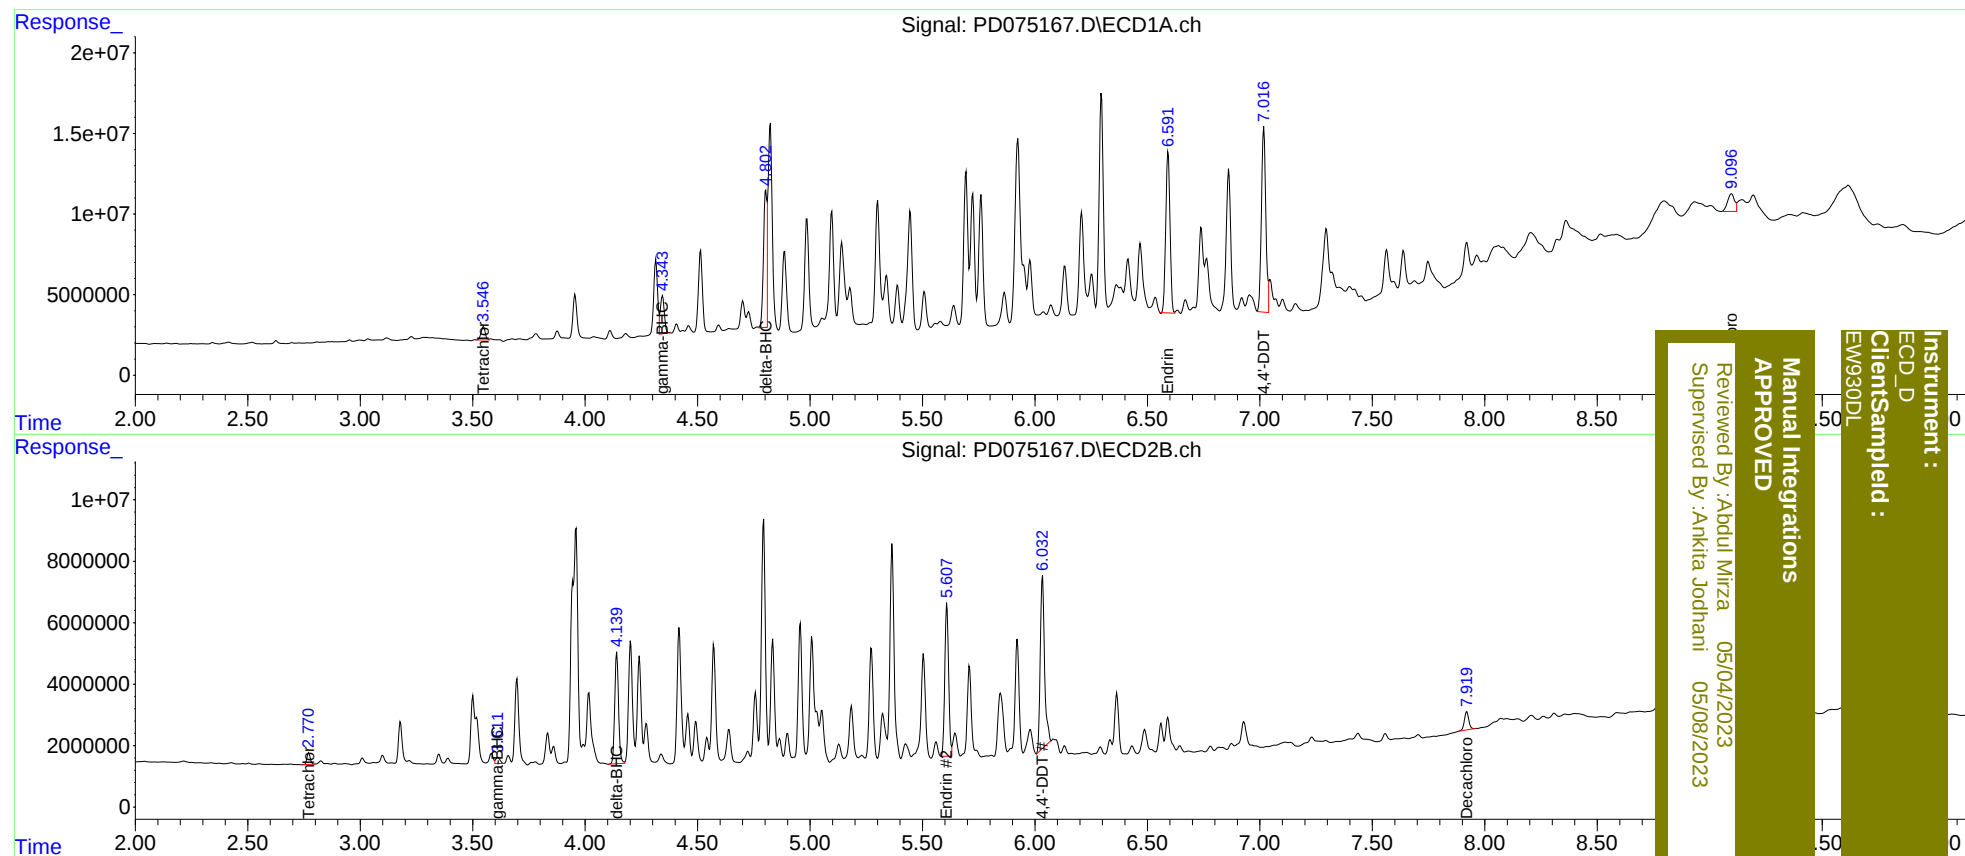

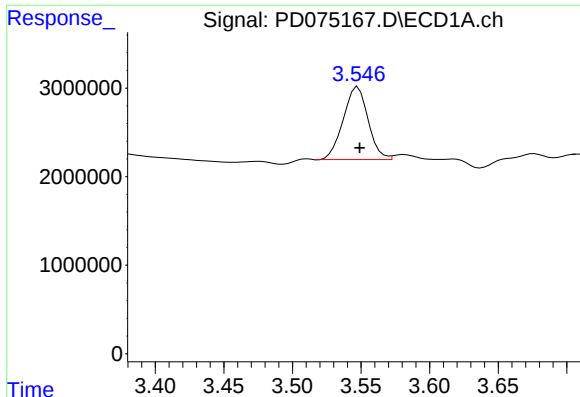


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: -0.001 min
Response: 10352776
Conc: 4.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW930DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/08/2023

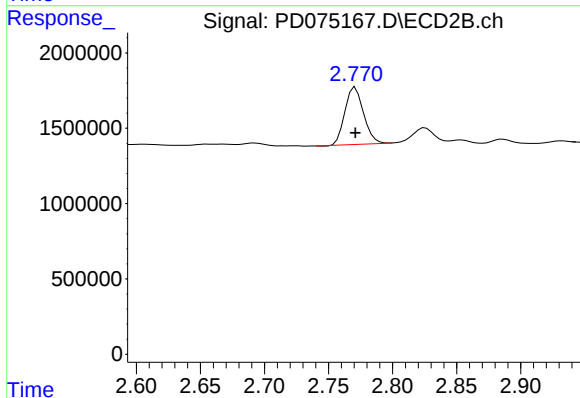


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 3841071
Conc: 3.64 ng/ml

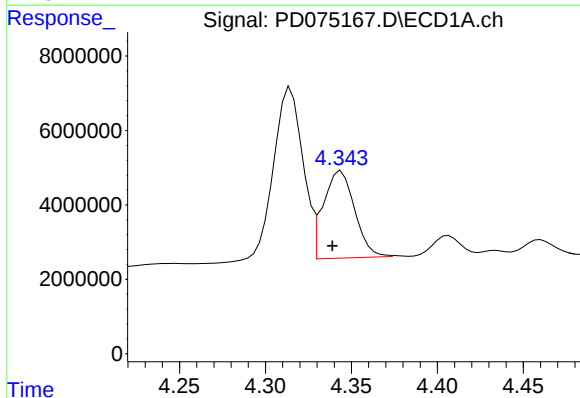


#3 gamma-BHC (Lindane)

R.T.: 4.343 min
Delta R.T.: 0.004 min
Response: 29000668
Conc: 8.07 ng/ml m

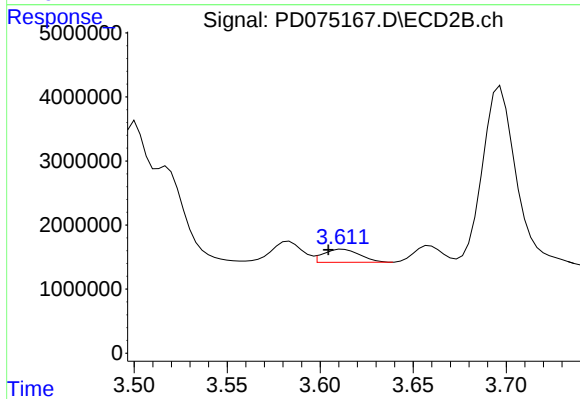

#3 gamma-BHC (Lindane)

R.T.: 3.612 min
Delta R.T.: 0.008 min
Response: 2764175
Conc: 1.88 ng/ml

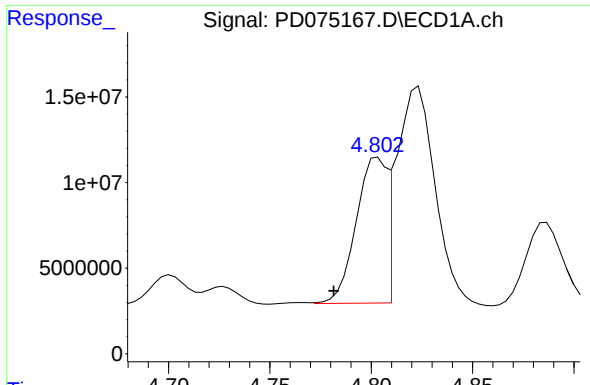


#7 delta-BHC

R.T.: 4.802 min
Delta R.T.: 0.020 min
Response: 109460017
Conc: 32.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW930DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/08/2023

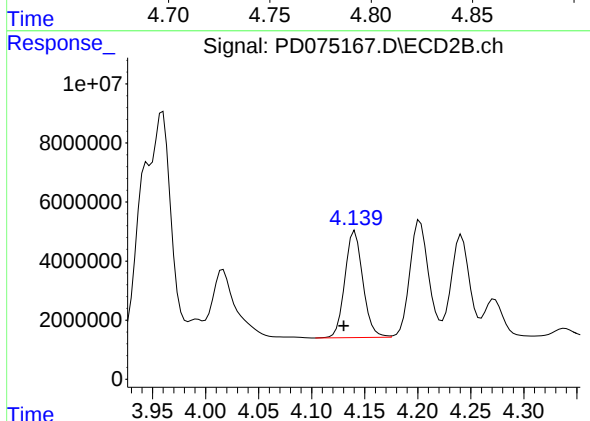


#7 delta-BHC

R.T.: 4.141 min
Delta R.T.: 0.010 min
Response: 42466254
Conc: 26.88 ng/ml

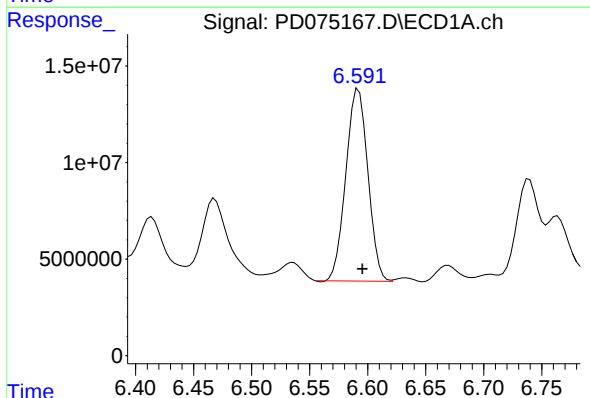


#14 Endrin

R.T.: 6.592 min
Delta R.T.: -0.003 min
Response: 131544038
Conc: 45.49 ng/ml

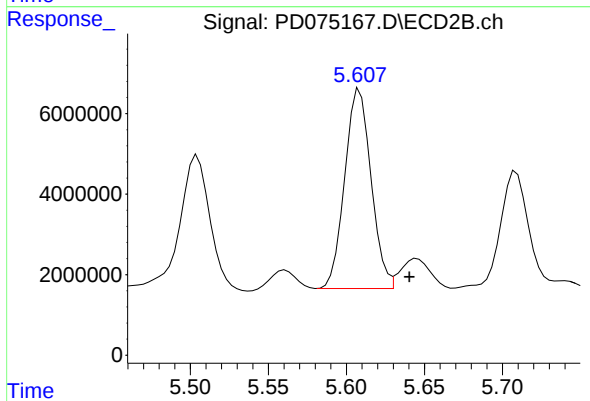

#14 Endrin

R.T.: 5.607 min
Delta R.T.: -0.033 min
Response: 59131515
Conc: 48.62 ng/ml m

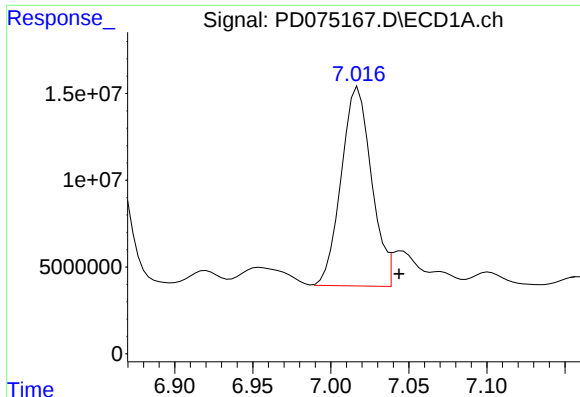


#17 4,4'-DDT

R.T.: 7.016 min
Delta R.T.: -0.028 min
Response: 154667768
Conc: 60.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW930DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/08/2023

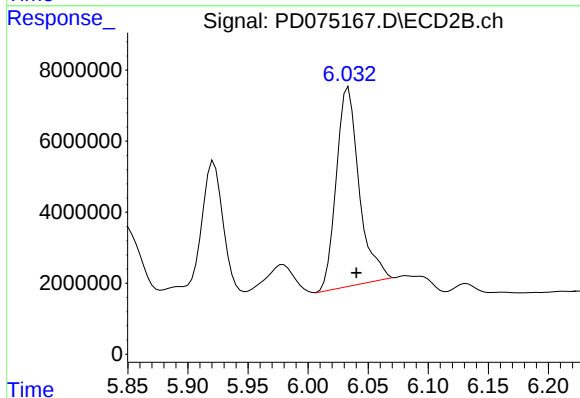


#17 4,4'-DDT

R.T.: 6.032 min
Delta R.T.: -0.008 min
Response: 74540069
Conc: 73.96 ng/ml m

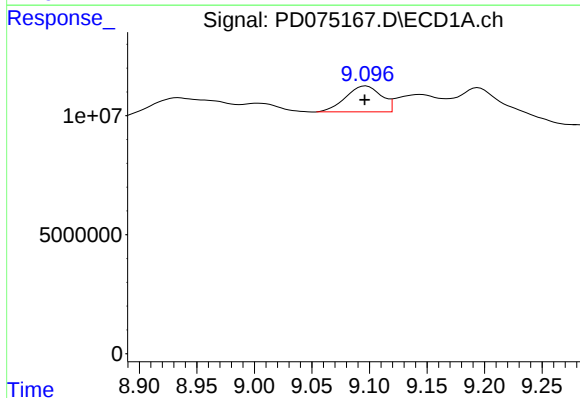

#27 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.000 min
Response: 22963586
Conc: 9.28 ng/ml m

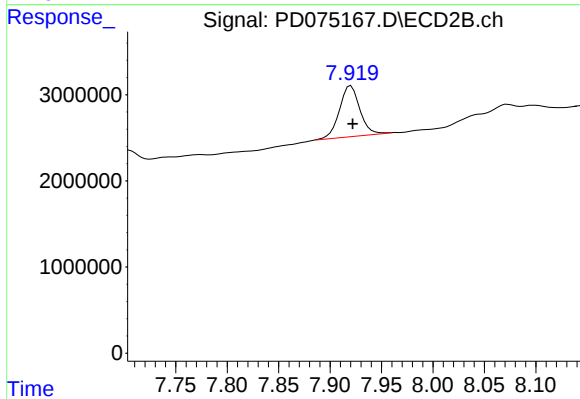

#27 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: -0.002 min
Response: 8244629
Conc: 8.73 ng/ml