

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
 Data File : PD075169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 19:42
 Operator : AR\AJ
 Sample : 02419-36DL2 100X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW931DL2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/04/2023
 Supervised By :Ankita Jodhani 05/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 02:57:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
7) B	delta-BHC	4.801	4.141	74886541	35508477	22.155m 22.472
14) MA	Endrin	6.591	5.607	175.2E6	74829188	60.579 61.521m
17) MA	4,4'-DDT	7.015	6.032	195.7E6	99569520	77.112m 98.792m#
19) B	Endosulfa...	7.155	6.333	7070750	5764820	2.570m 4.957m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
Data File : PD075169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2023 19:42
Operator : AR\AJ
Sample : 02419-36DL2 100X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 02:57:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

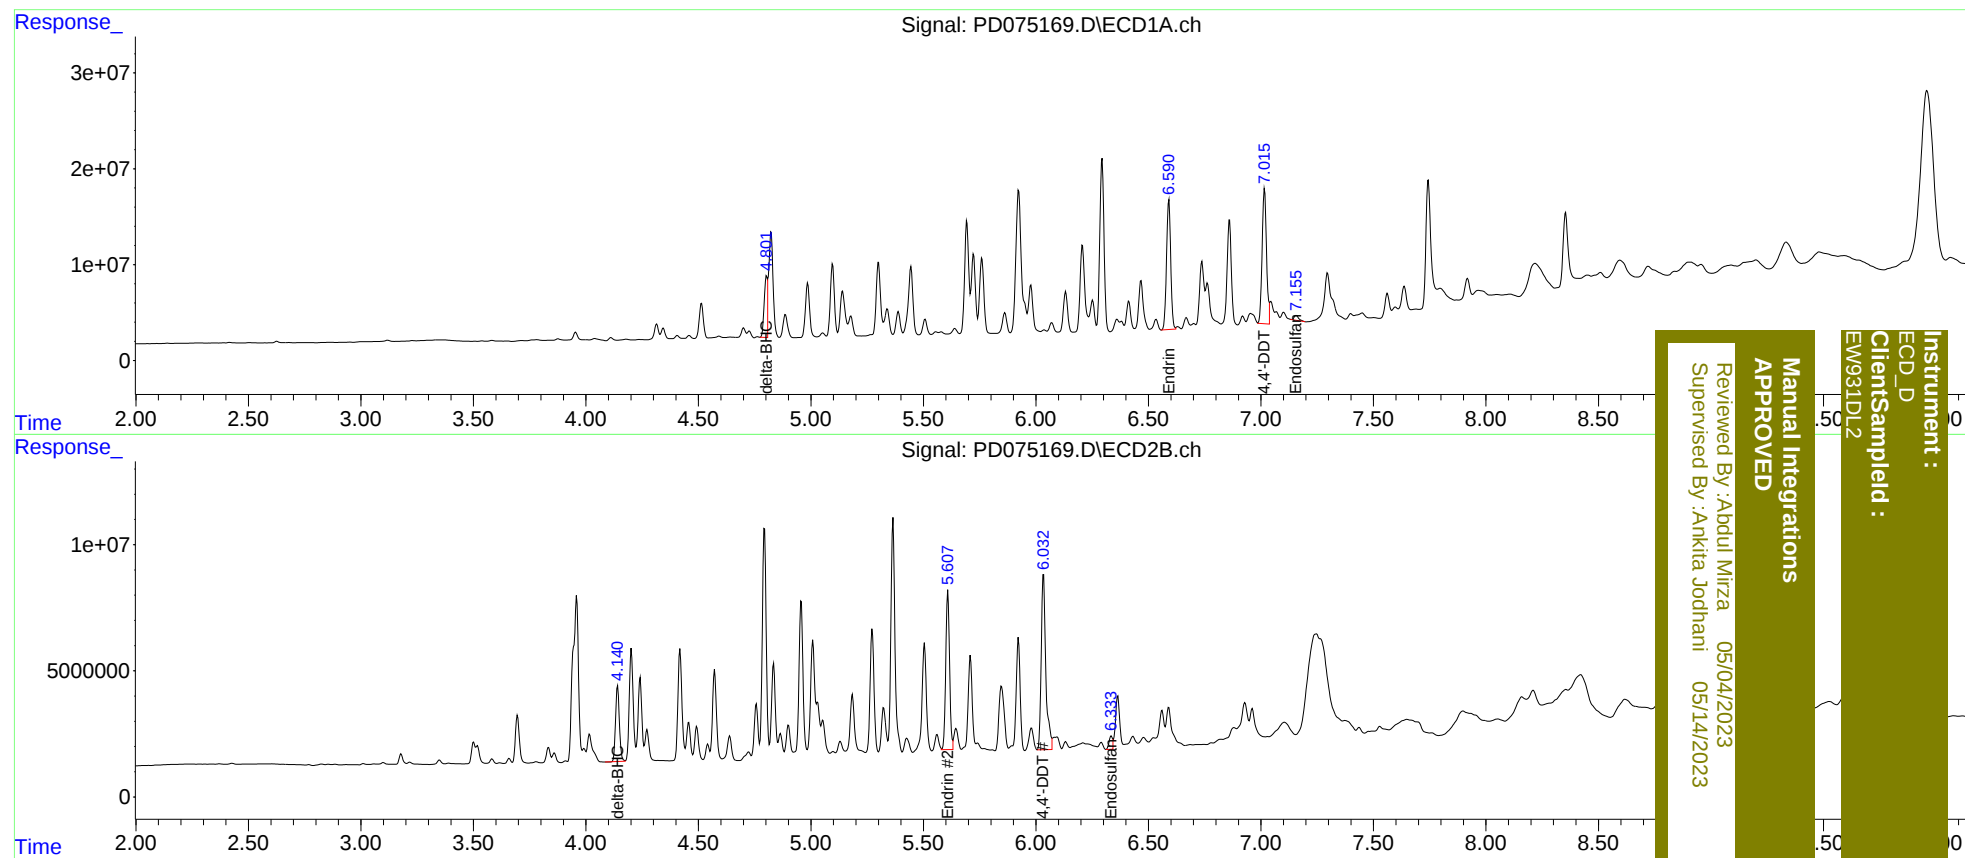

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/14/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW/931DL2

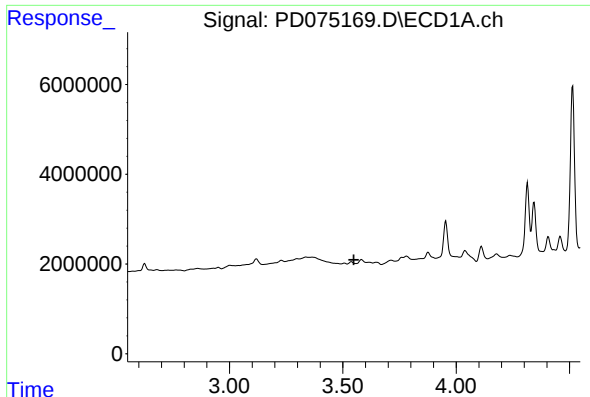


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EW931DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/14/2023

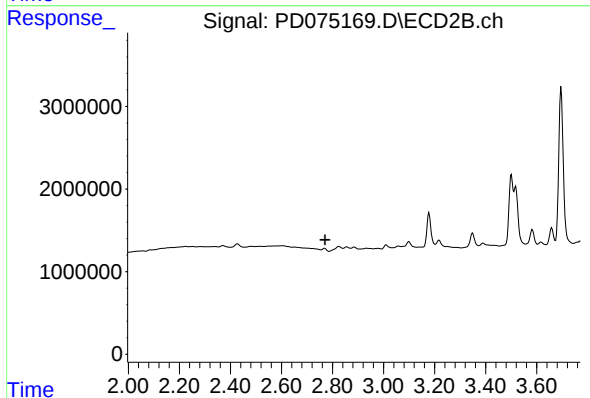


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.771 min
Response: 0
Conc: N.D.

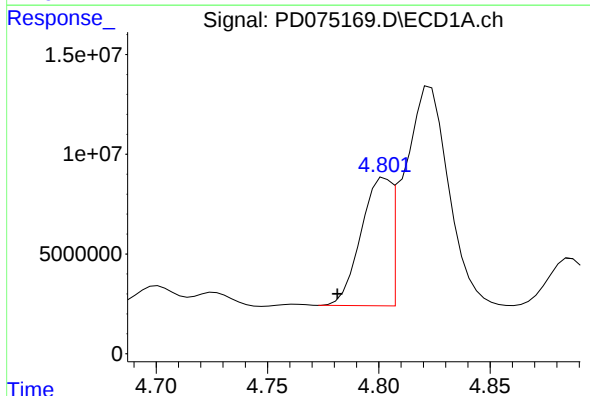


#7 delta-BHC

R.T.: 4.801 min
Delta R.T.: 0.020 min
Response: 74886541
Conc: 22.15 ng/ml m

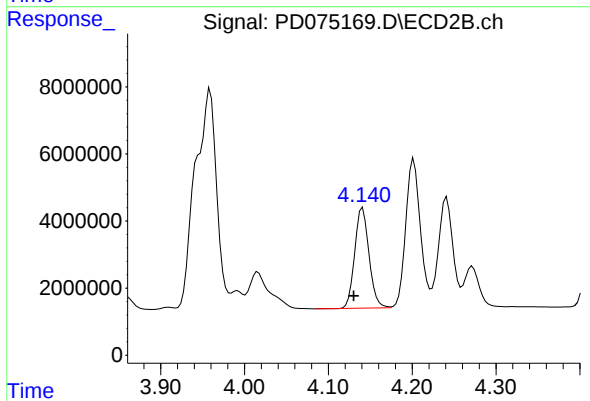

#7 delta-BHC

R.T.: 4.141 min
Delta R.T.: 0.011 min
Response: 35508477
Conc: 22.47 ng/ml

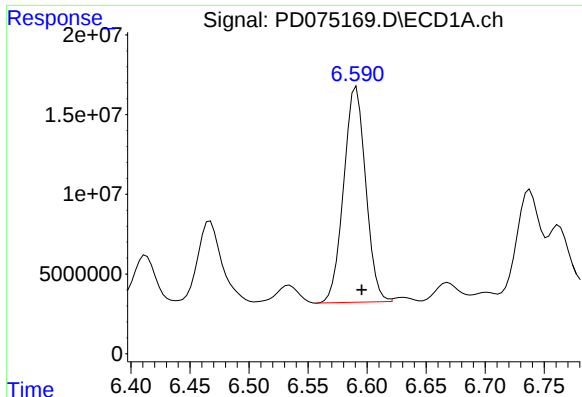


#14 Endrin

R.T.: 6.591 min
Delta R.T.: -0.004 min
Response: 175183205
Conc: 60.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW931DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/14/2023

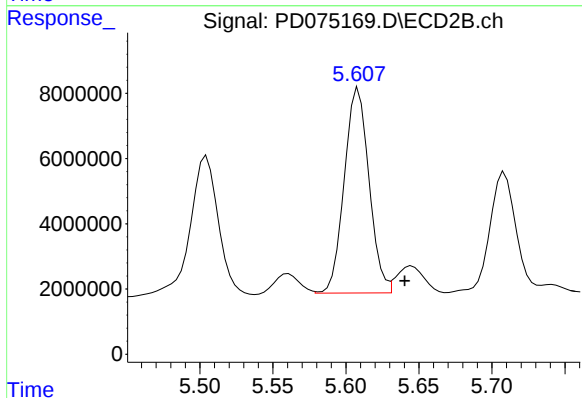


#14 Endrin

R.T.: 5.607 min
Delta R.T.: -0.033 min
Response: 74829188
Conc: 61.52 ng/ml m

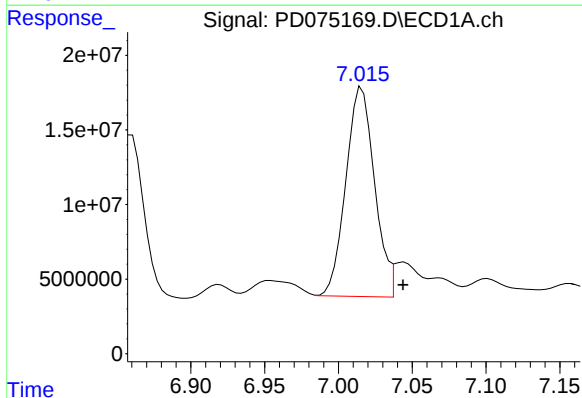


#17 4,4'-DDT

R.T.: 7.015 min
Delta R.T.: -0.029 min
Response: 195728078
Conc: 77.11 ng/ml m

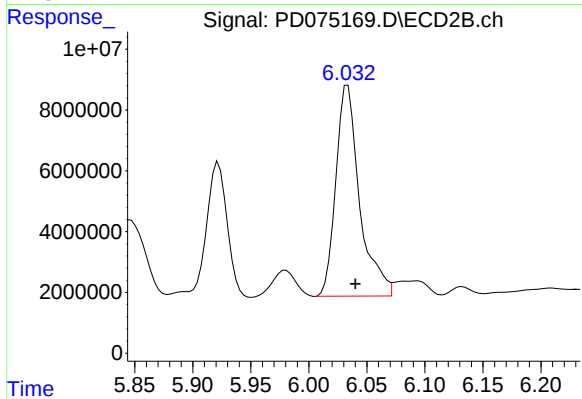

#17 4,4'-DDT

R.T.: 6.032 min
Delta R.T.: -0.008 min
Response: 99569520
Conc: 98.79 ng/ml m

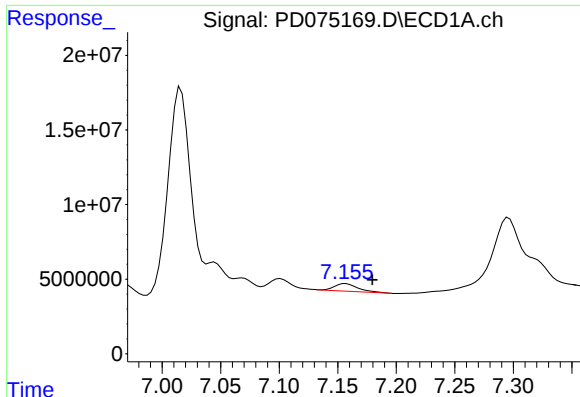


#19 Endosulfan Sulfate

R.T.: 7.155 min
Delta R.T.: -0.024 min
Response: 7070750
Conc: 2.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
EW931DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/04/2023
Supervised By :Ankita Jodhani 05/14/2023

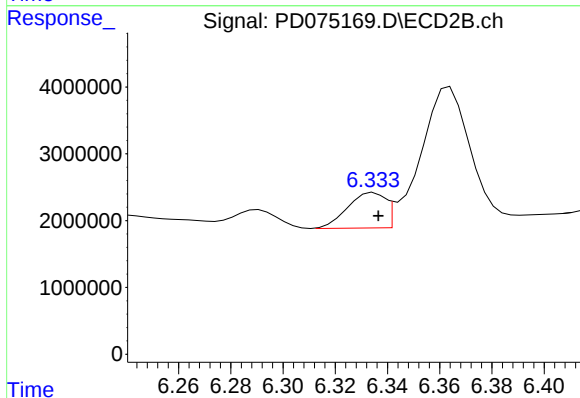


#19 Endosulfan Sulfate

R.T.: 6.333 min
Delta R.T.: -0.003 min
Response: 5764820
Conc: 4.96 ng/ml m

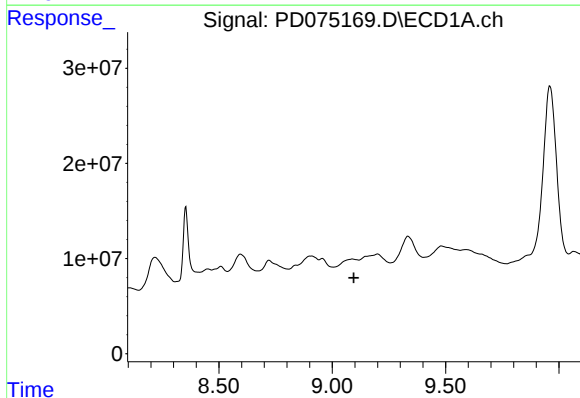

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

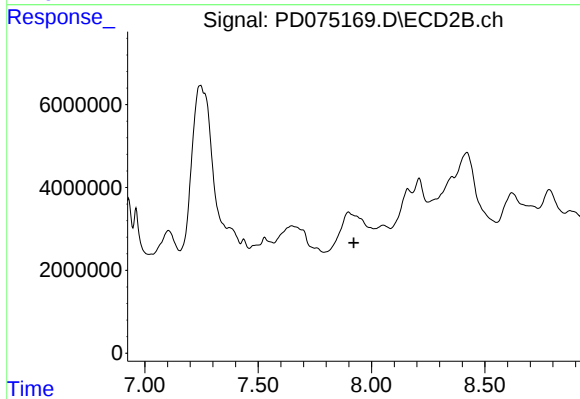

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.922 min
Response: 0
Conc: N.D.