

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
 Data File : PD075178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 21:44
 Operator : AR\AJ
 Sample : 02417-08DL 20X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW8X4DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/04/2023
 Supervised By : Ankita Jodhani 05/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 02:59:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	9.095	7.919	3501217	1954220	1.415	2.069m#
Target Compounds							
4)	MA Heptachlor	4.931	3.945	1024.2E6	378.9E6	274.735	259.316
5)	MB Aldrin	5.272	4.225	541.0E6	195.0E6	148.331m	131.469
6)	B beta-BHC	4.532	3.903	1023553	601039	0.624m	0.825m#
8)	B Heptachlo...	5.701	4.728	400.8E6	139.8E6	118.261	100.218
10)	B trans-Chl...	5.958	4.978	1053.0E6	437.5E6	321.361	320.640
11)	B cis-Chlor...	6.039	5.042	327.6E6	91928280	96.126	65.871 #
12)	B 4,4'-DDE	6.207	5.231	36288916	11199647	11.113	8.712
13)	MA Dieldrin	6.364	5.363	2978.7E6	1098.6E6	871.028	805.188
14)	MA Endrin	6.594	5.647	12547870	13759739	4.339m	11.313 #
16)	A 4,4'-DDD	6.726	5.785	24348728	11023219	10.076m	11.119m
17)	MA 4,4'-DDT	7.042	6.038	94606563	37296746	37.272	37.006
21)	B Endrin ke...	7.665	6.841	111.7E6	48054808	36.841	36.443m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
 Data File : PD075178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2023 21:44
 Operator : AR\AJ
 Sample : 02417-08DL 20X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 02:59:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

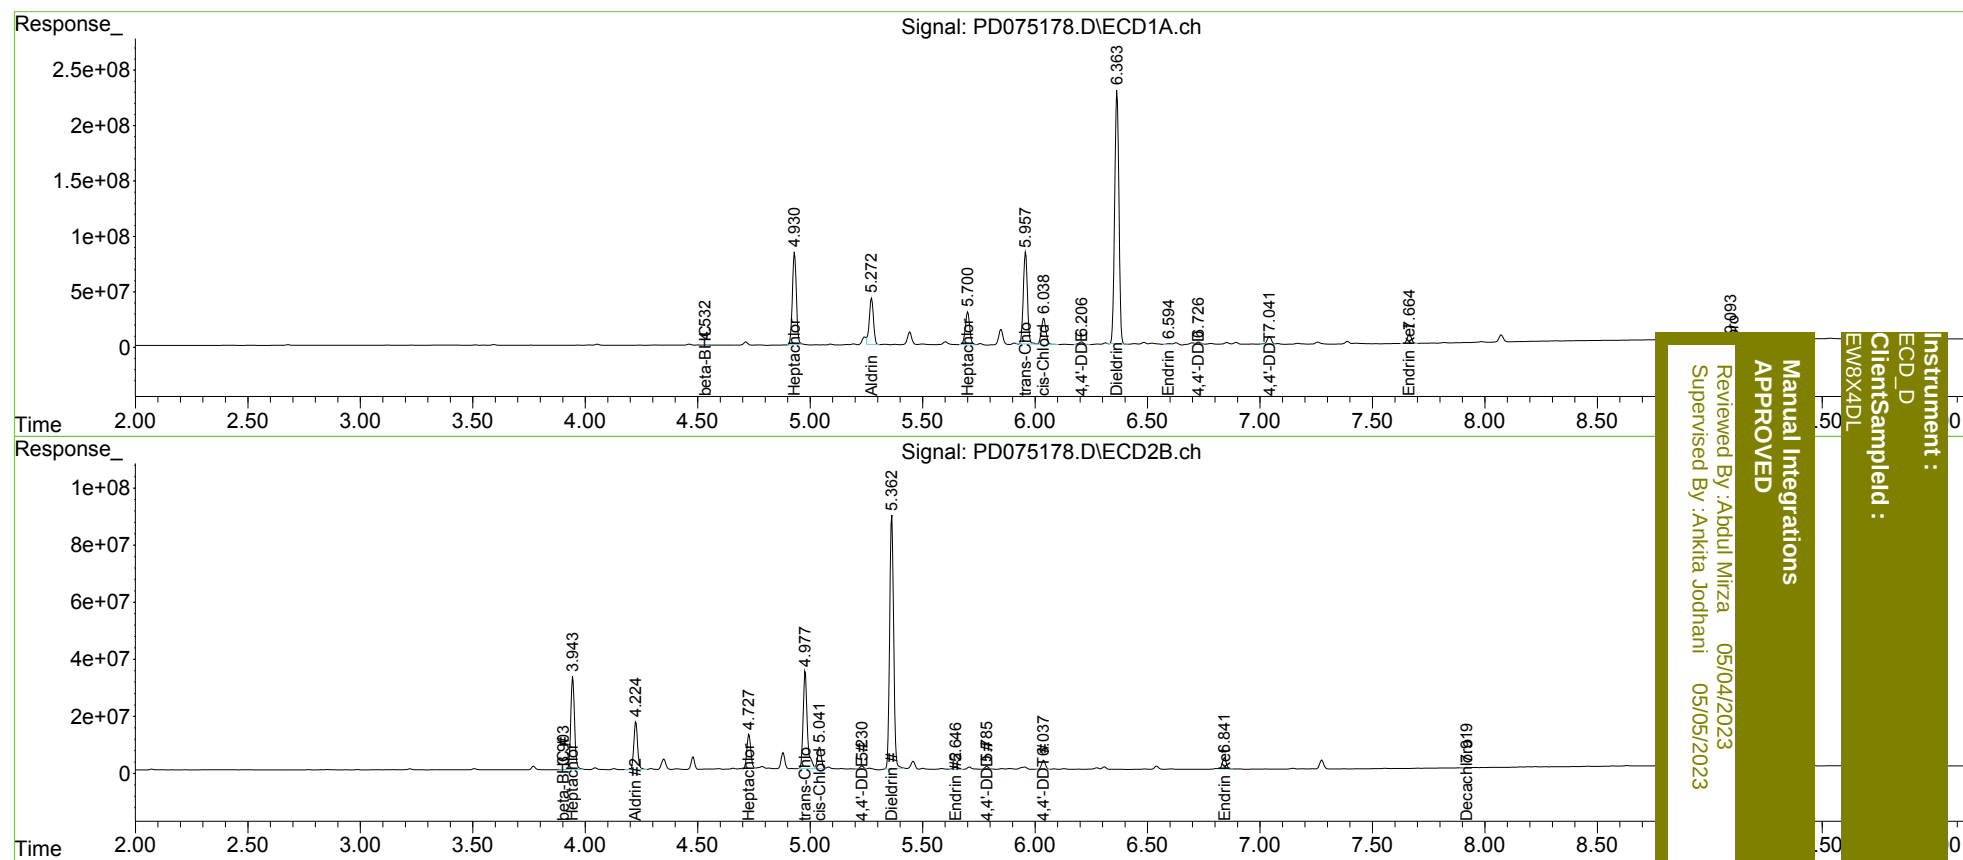

Instrument :
 ECD_D
 ClientSampled :
 EW8X4DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/04/2023
 Supervised By :Ankita Jodhani 05/05/2023