

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
 Data File : PD075187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 00:40
 Operator : AR\AJ
 Sample : 02447-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW911

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/06/2023
 Supervised By : Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 03:00:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.771	30988284	14913251	13.586	14.139
27)	SA Decachlor...	9.092	7.919	70867491	20062290	28.637m	21.244 #
Target Compounds							
3)	MA gamma-BHC...	4.342	3.609	3562117	6420362	0.991m	4.368 #
7)	B delta-BHC	4.801	4.141	18986938	14363806	5.617m	9.090 #
14)	MA Endrin	6.591	5.607	42029529	20711582	14.534	17.028m
17)	MA 4,4'-DDT	7.014	6.032	50368161	26113436	19.844m	25.910m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050323\
Data File : PD075187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 00:40
Operator : AR\AJ
Sample : 02447-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 03:00:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

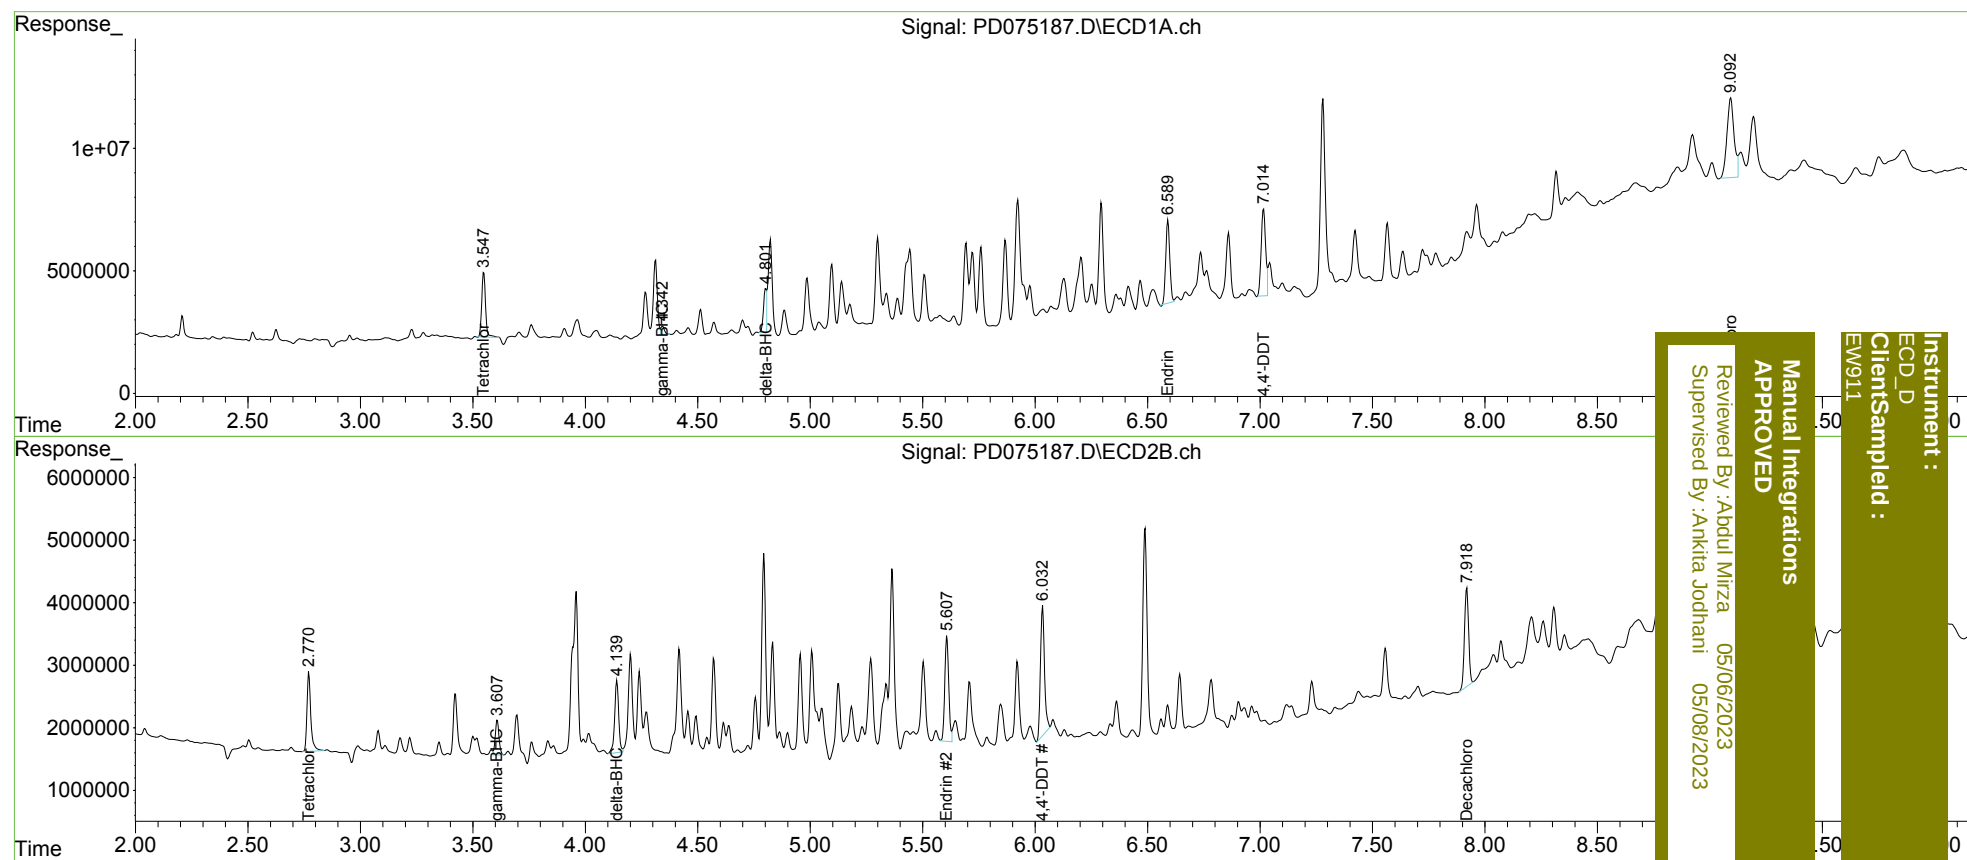

Reviewed By: Abdul Mirza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW/11