

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
Data File : PD062687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 13:06
Operator : AR\AJ
Sample : M2243-07
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PEST-GPC-BLANK-SPIKE

Manual Integrations
APPROVED

Ankita
5/5/2021 10:28:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 01:30:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

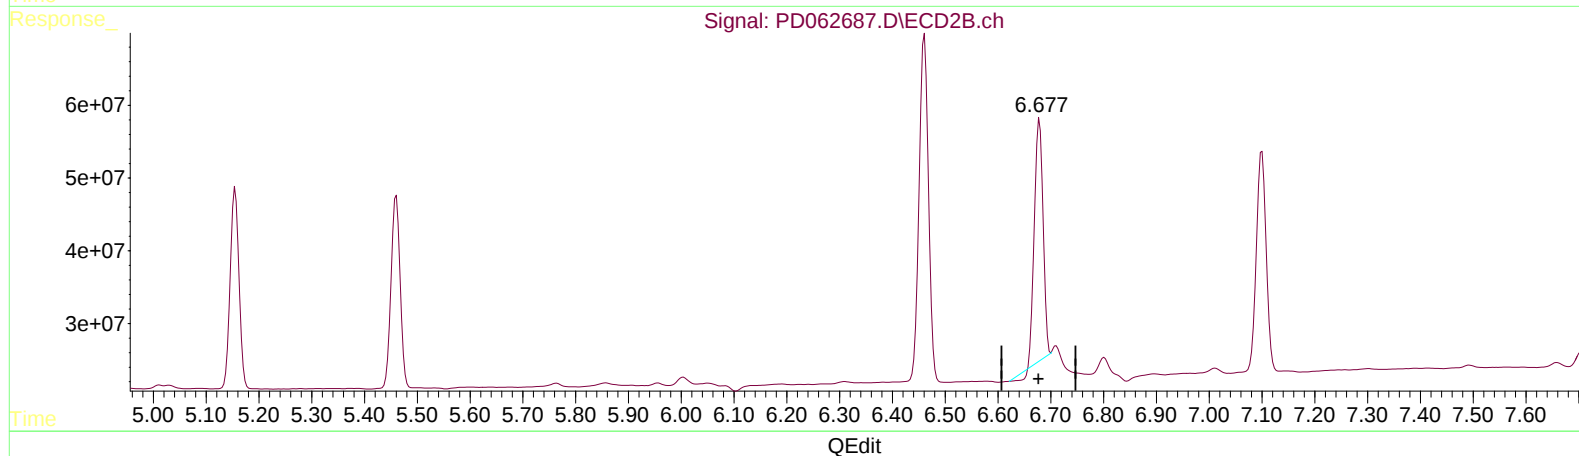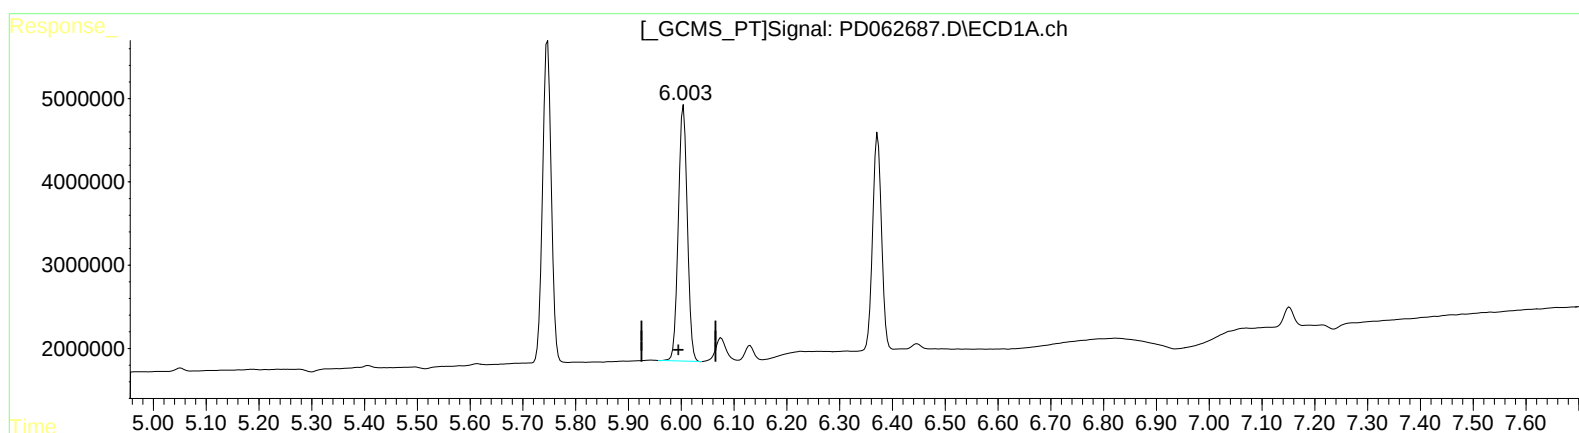

(14) Endrin (MA)

6.004min 34.382 ng/ml

response 36379467

(14) Endrin #2 (MA)

6.679min 29.741 ng/ml

response 370911945

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
Data File : PD062687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 13:06
Operator : AR\AJ
Sample : M2243-07
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PEST-GPC-BLANK-SPIKE

Manual Integrations
APPROVED

Ankita
5/5/2021 10:28:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 01:30:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

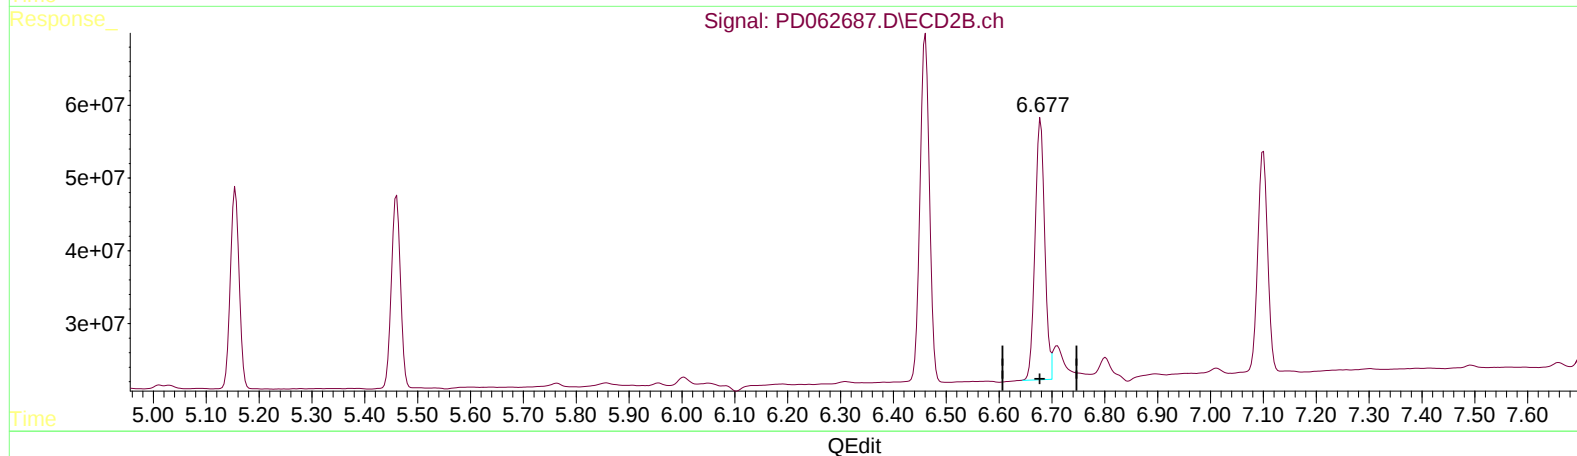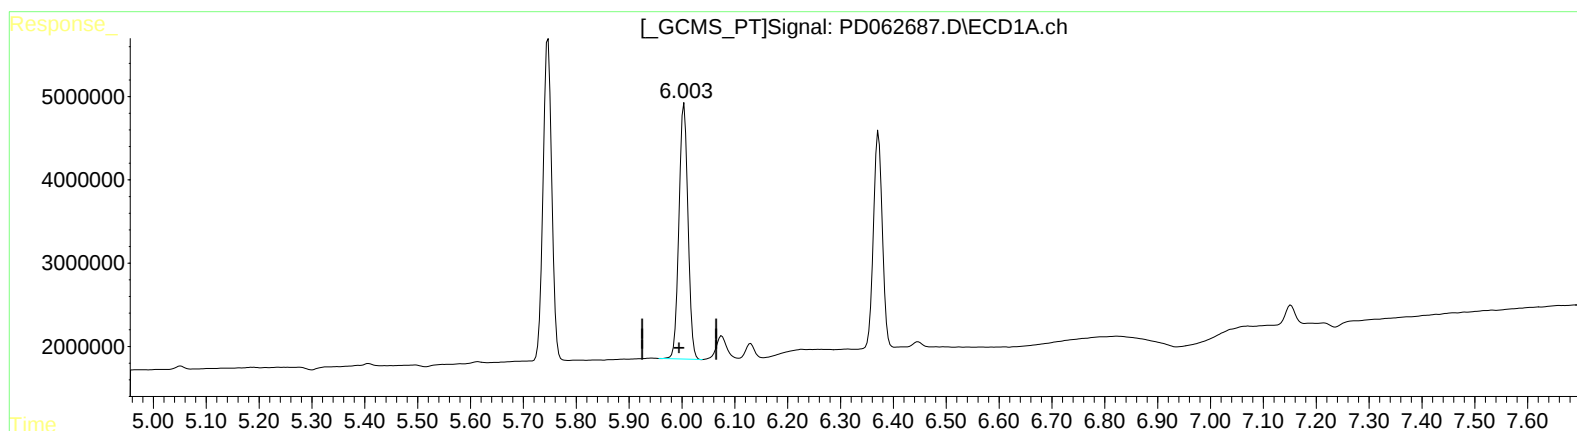

(14) Endrin (MA)

6.004min 34.382 ng/ml

response 36379467

(14) Endrin #2 (MA)

6.677min 36.146 ng/ml m

response 450796990

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
 Data File : PD062687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2021 13:06
 Operator : AR\AJ
 Sample : M2243-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEST-GPC-BLANK-SPIKE

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:28:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 01:30:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) MA	gamma-BHC...	4.170	4.647	23761609	350.3E6	17.788	20.277
4) MA	Heptachlor	4.472	5.155	21987626	322.0E6	17.124	18.500
5) MB	Aldrin	4.721	5.460	21758704	320.6E6	16.704	18.536
13) MA	Dieldrin	5.747	6.461	44640142	594.4E6	35.414	38.335
14) MA	Endrin	6.004	6.677	36379467	450.8E6	34.382	36.146m
17) MA	4,4'-DDT	6.372	7.100	30325133	395.8E6	32.376	33.336

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AD
 5/5/21