

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
 Data File : PD062700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2021 17:12
 Operator : AR\AJ
 Sample : M2232-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5A3

Manual Integrations
 APPROVED

Ankita
 5/7/2021 1:57:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 01:35:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	3.972	12690884	151.8E6	13.256	12.498
27)	SA Decachlor...	8.203	9.032	25661114	291.6E6	23.907	26.715m
Target Compounds							
10)	B trans-Chl...	5.383	6.081	978078	25586072	0.780	1.562m#
11)	B cis-Chlor...	5.439	6.151	1499400	34497869	1.221m	2.222m#
12)	B 4,4'-DDE	5.603	6.304	377965	41238501	0.305m	2.632m#
13)	MA Dieldrin	5.736	6.460	7535699	8750221	5.978m	0.564m#
16)	A 4,4'-DDD	6.122	6.797	1532570	66012812	1.539m	5.311 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
Data File : PD062700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 17:12
Operator : AR\AJ
Sample : M2232-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:35:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

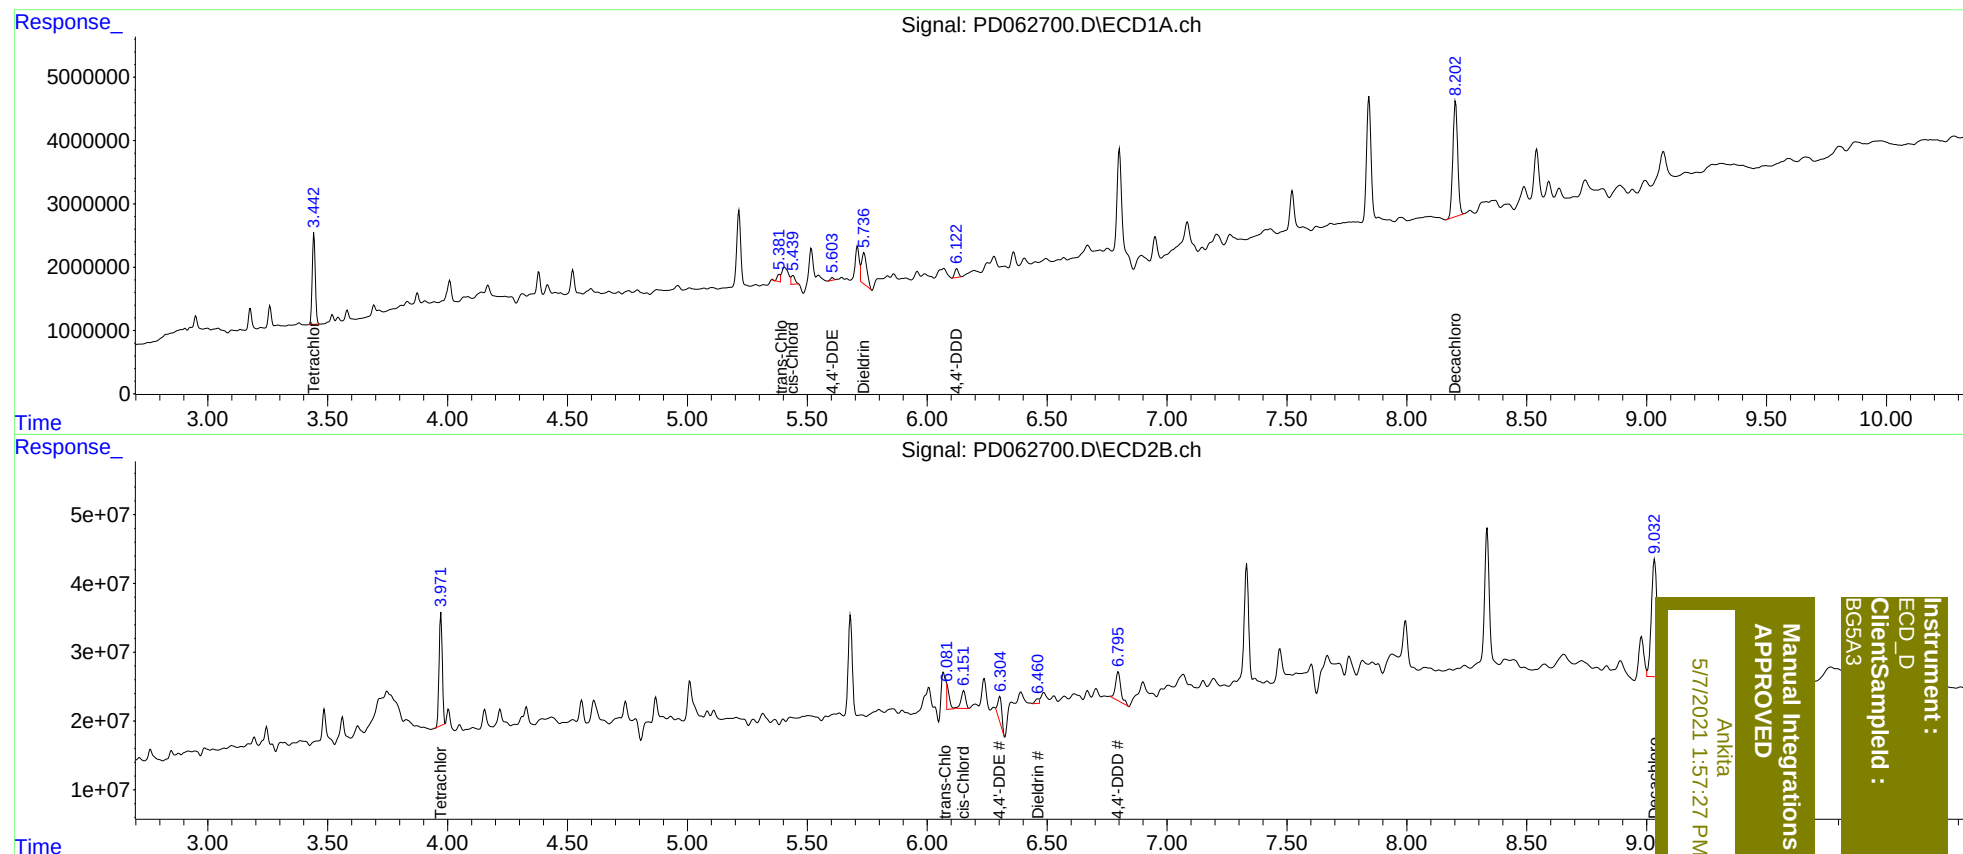

Manual Integrations
APPROVED

Ankita
5/7/2021 1:57:27 PM

Instrument :
ECD_D
ClientSampled :
BG5A3