

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
 Data File : PD062702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2021 17:40
 Operator : AR\AJ
 Sample : M2232-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5A9

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:28:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 01:34:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	3.958	8098442	2163.1E6	8.459	178.132m#
27)	SA Decachlor...	8.203	9.034	13433458	145.5E6	12.515	13.333
Target Compounds							
10)	B trans-Chl...	5.387	6.081	1289290	33157413	1.028m	2.025m#
11)	B cis-Chlor...	5.439	6.153	819600	16836949	0.667	1.085 #
12)	B 4,4'-DDE	5.603	6.306	256344	13037211	0.207m	0.832 #
13)	MA Dieldrin	5.736	6.460	936748	7061487	0.743m	0.455m#
16)	A 4,4'-DDD	6.120	6.800	864516	22035020	0.868m	1.773m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
Data File : PD062702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 17:40
Operator : AR\AJ
Sample : M2232-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 01:34:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

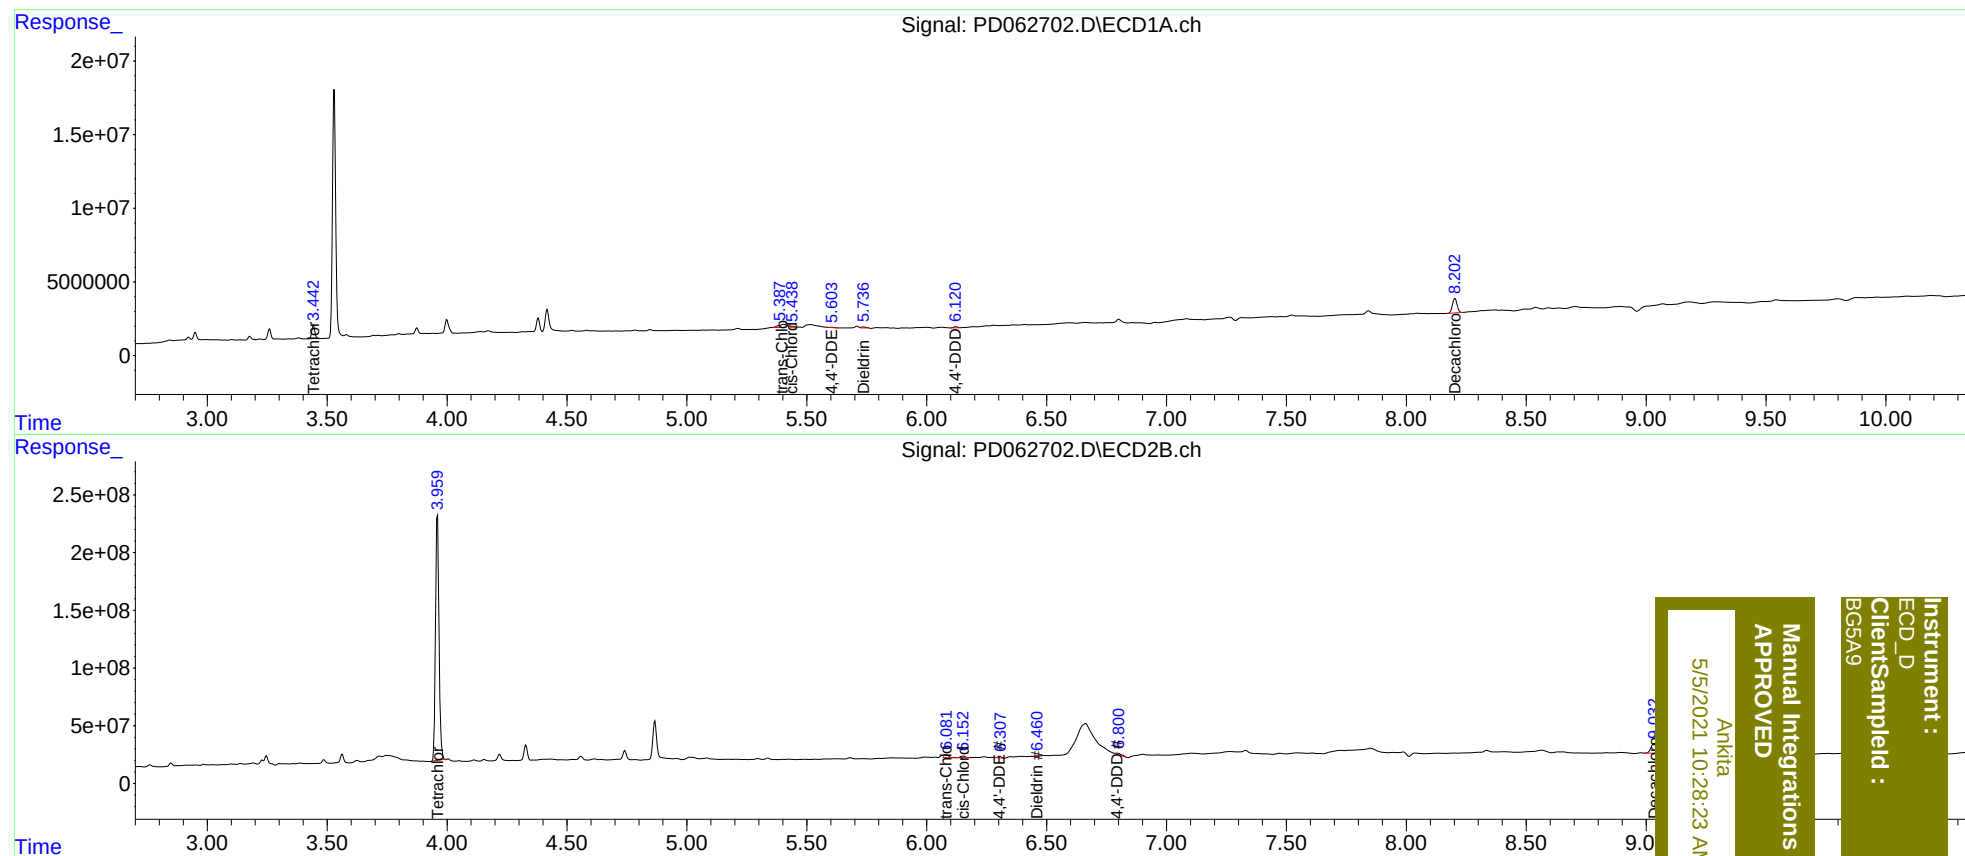

Manual Integrations
APPROVED

Ankita
5/5/2021 10:28:23 AM

Instrument :
ECD_D
ClientSampleId :
BG5A9