

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
 Data File : PD062706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2021 18:35
 Operator : AR\AJ
 Sample : 10 PPB SPIKE
 Misc : PP18453
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 10 PPB SPIKE

Manual Integrations
 APPROVED

Ankita
 5/5/2021 10:28:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 01:35:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
Target Compounds						
2) A alpha-BHC	3.880	4.362	11286112	179.9E6	8.061	9.511
3) MA gamma-BHC...	4.163	4.646	11052266	164.0E6	8.274	9.494
4) MA Heptachlor	4.464	5.154	10919493	169.1E6	8.504	9.719
5) MB Aldrin	4.713	5.459	10753467	165.6E6	8.256	9.576
6) B beta-BHC	4.414	4.817	5664486	71630770	9.124	9.383
7) B delta-BHC	4.618	5.031	8602276	150.7E6	6.322	8.122m#
8) B Heptachlo...	5.156	5.845	10574285	154.9E6	8.629	9.658
9) A Endosulfan I	5.495	6.201	9734369	140.2E6	8.706	9.560
10) B trans-Chl...	5.383	6.079	10498693	152.4E6	8.374	9.304
11) B cis-Chlor...	5.442	6.152	10407298	147.6E6	8.475	9.509
12) B 4,4'-DDE	5.606	6.309	9953834	149.4E6	8.043	9.536
13) MA Dieldrin	5.739	6.458	10317938	152.0E6	8.185	9.800
14) MA Endrin	5.997	6.676	8803123	113.7E6	8.320	9.117
15) B Endosulfa...	6.270	6.886	8905820	120.8E6	8.587	9.649
16) A 4,4'-DDD	6.123	6.798	8538549	127.2E6	8.575	10.237
17) MA 4,4'-DDT	6.364	7.097	6351147	103.2E6	6.781	8.690 #
18) B Endrin al...	6.440	7.010	7583000	98845487	8.499	9.060
19) B Endosulfa...	6.653	7.233	8586067	117.3E6	8.589	9.193
20) A Methoxychlor	6.910	7.557	3833745	50772712	7.185	8.958
21) B Endrin ke...	7.145	7.703	10511871	120.7E6	8.970	9.804

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050421\
Data File : PD062706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2021 18:35
Operator : AR\AJ
Sample : 10 PPB SPIKE
Misc : PP18453
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 01:35:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

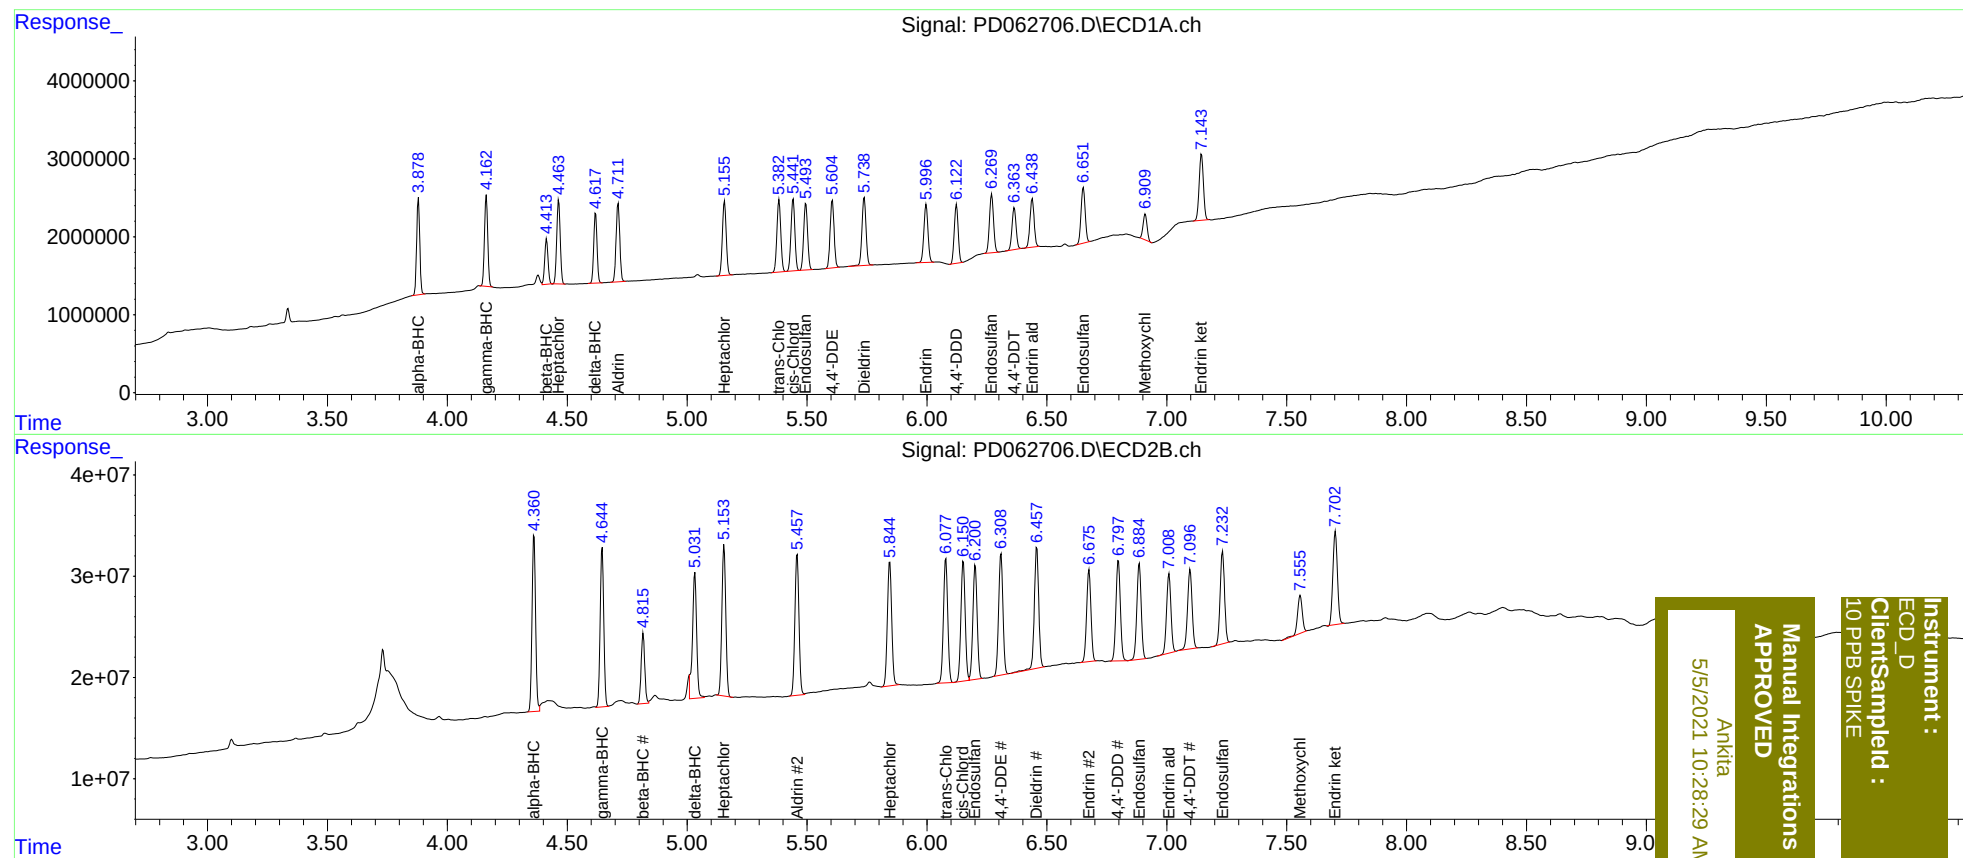

Manual Integrations
APPROVED

5/5/2021 10:28:29 AM

Ankita

Instrument :
ECD_D
ClientSampled :
10 PPB SPIKE