

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
 Data File : PD075252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 09:24
 Operator : AR\AJ
 Sample : 02561-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 02:19:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.587f	0.000	146861	0	<MDL	N.D. #
27)	SA Decachlor...	9.097	0.000	3253257	0	1.315	N.D. #
Target Compounds							
2)	A alpha-BHC	4.004	0.000	146738	0	<MDL	N.D. #
3)	MA gamma-BHC...	4.325	0.000	21243	0	<MDL	N.D. #
7)	B delta-BHC	4.773	4.152	740762	-215253	0.219	N.D. #
8)	B Heptachlo...	5.698	0.000	1432002	0	0.423	N.D. #
10)	B trans-Chl...	5.927	0.000	49879	0	<MDL	N.D. #
13)	MA Dieldrin	6.433f	0.000	398714	0	0.117	N.D. #
17)	MA 4,4'-DDT	7.023	0.000	2475014	0	0.975	N.D. #
20)	A Methoxychlor	0.000	6.640	0	658505	N.D.	1.150
23)	Toxaphene-2	6.489	0.000	179151	0	6.004	N.D. #
25)	Toxaphene-4	0.000	6.640	0	658505	N.D.	26.010

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
Data File : PD075252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 09:24
Operator : AR\AJ
Sample : 02561-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 02:19:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

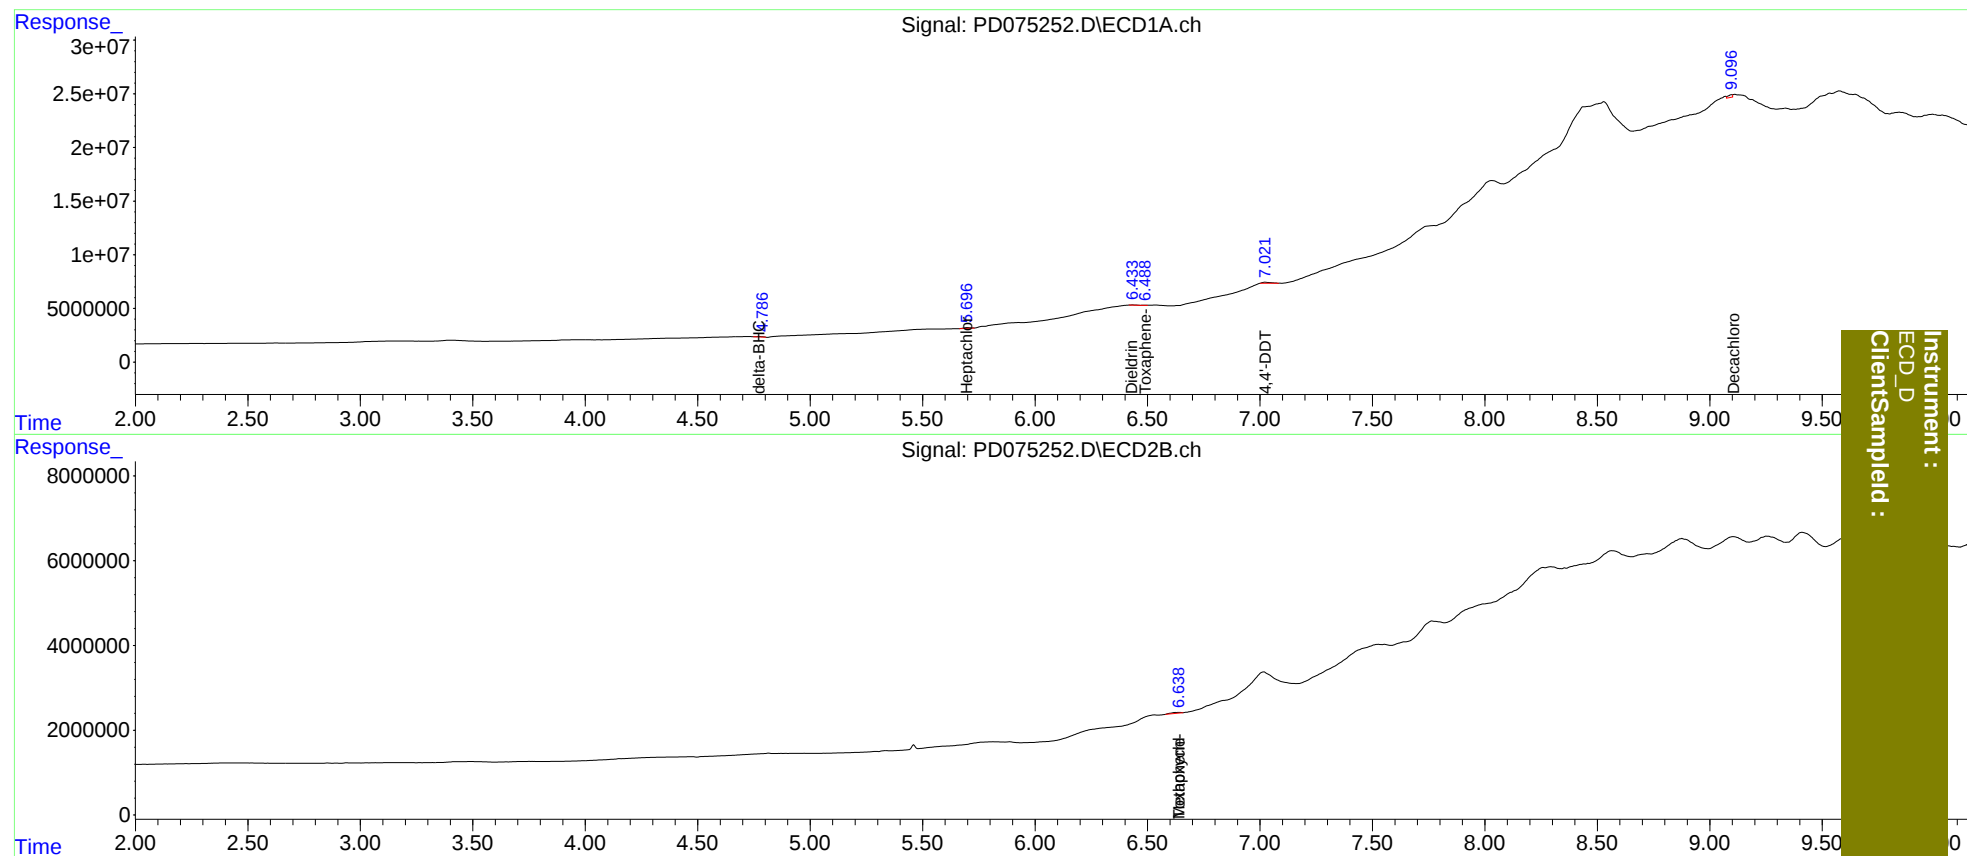


Instrument :
ECD_D
ClientSampled :
0

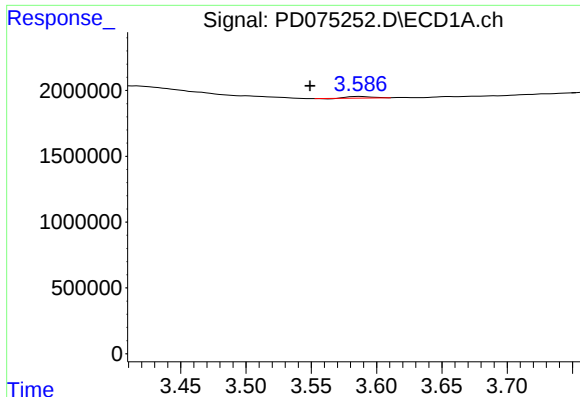

#1 Tetrachloro-m-xylene


R.T.: 3.587 min
Delta R.T.: 0.038 min
Response: 146861
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

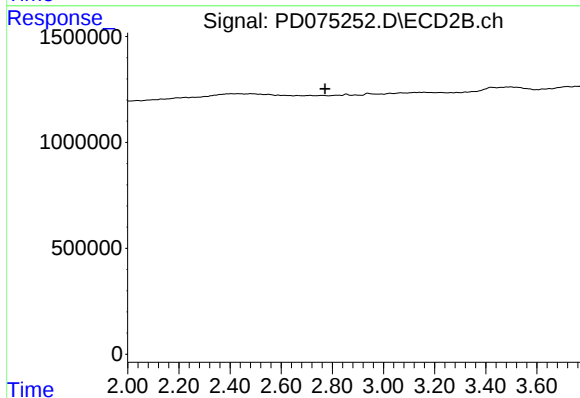


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.771 min
Response: 0
Conc: N.D.

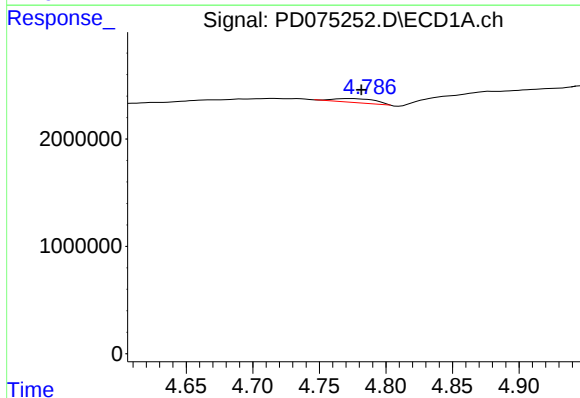


#7 delta-BHC

R.T.: 4.773 min
Delta R.T.: -0.009 min
Response: 740762
Conc: 0.22 ng/ml

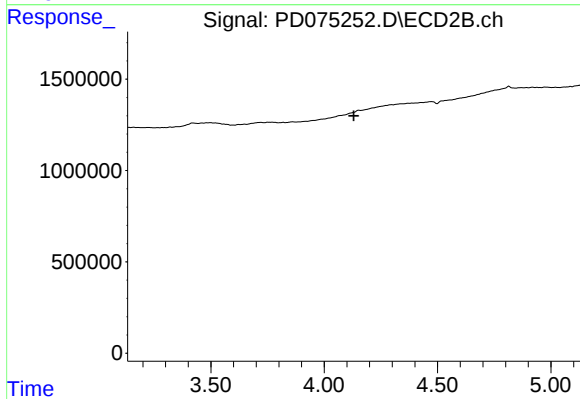

#7 delta-BHC


R.T.: 4.152 min
Delta R.T.: 0.021 min
Response: -215253
Conc: N.D.

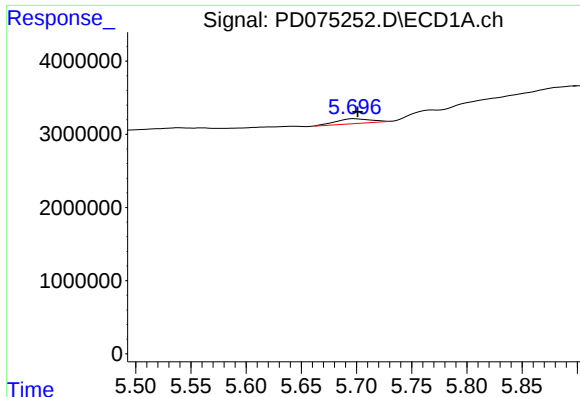

#8 Heptachlor epoxide


R.T.: 5.698 min
Delta R.T.: -0.003 min
Response: 1432002
Conc: 0.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

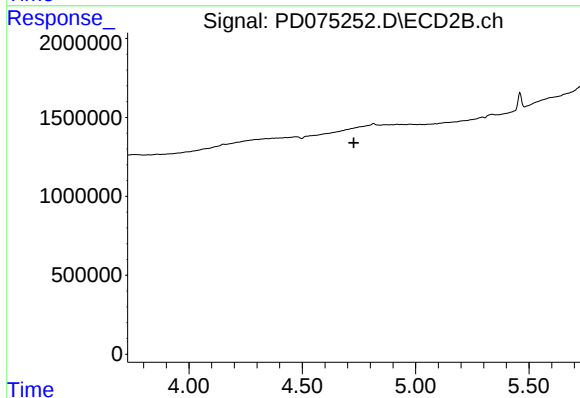


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.728 min
Response: 0
Conc: N.D.

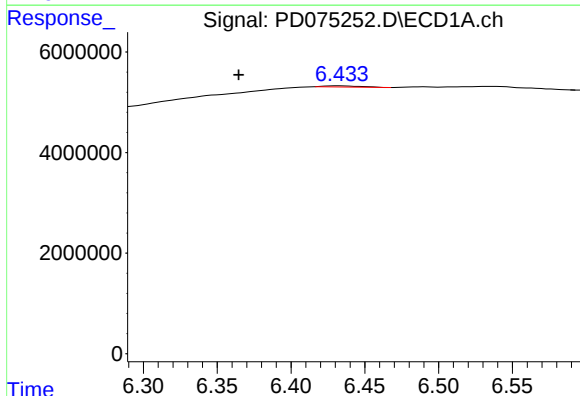


#13 Dieldrin

R.T.: 6.433 min
Delta R.T.: 0.068 min
Response: 398714
Conc: 0.12 ng/ml

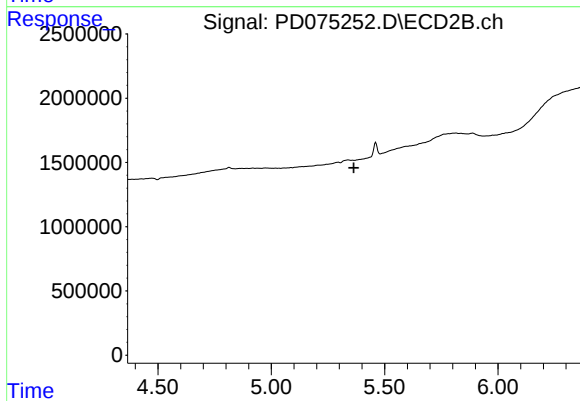

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.364 min
Response: 0
Conc: N.D.

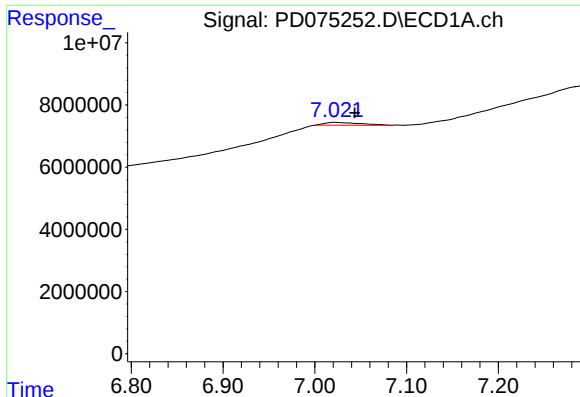

#17 4,4'-DDT


R.T.: 7.023 min
Delta R.T.: -0.021 min
Response: 2475014
Conc: 0.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

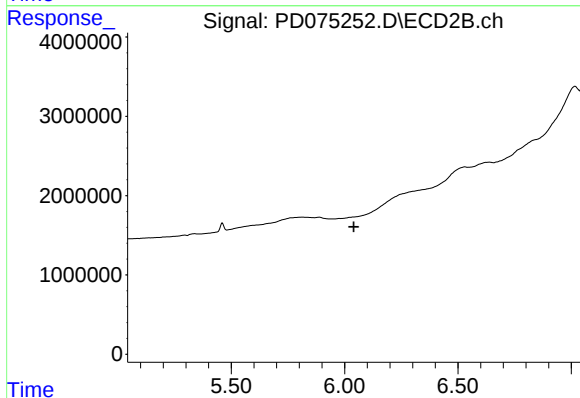


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.040 min
Response: 0
Conc: N.D.

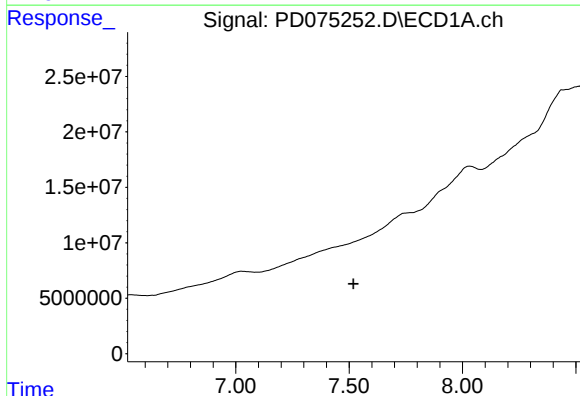


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.520 min
Response: 0
Conc: N.D.

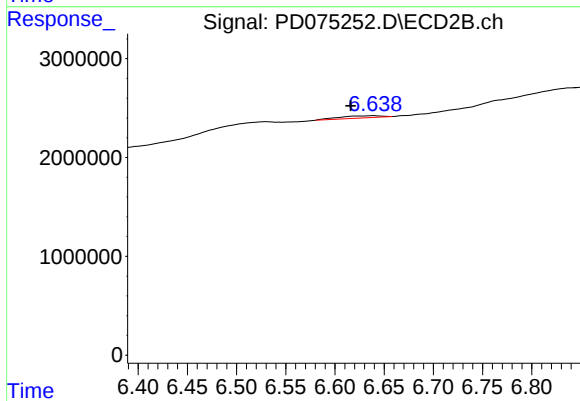

#20 Methoxychlor


R.T.: 6.640 min
Delta R.T.: 0.023 min
Response: 658505
Conc: 1.15 ng/ml

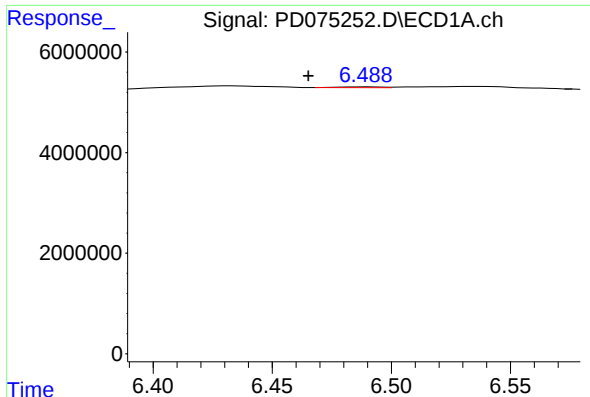

#23 Toxaphene-2


R.T.: 6.489 min
Delta R.T.: 0.024 min
Response: 179151
Conc: 6.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

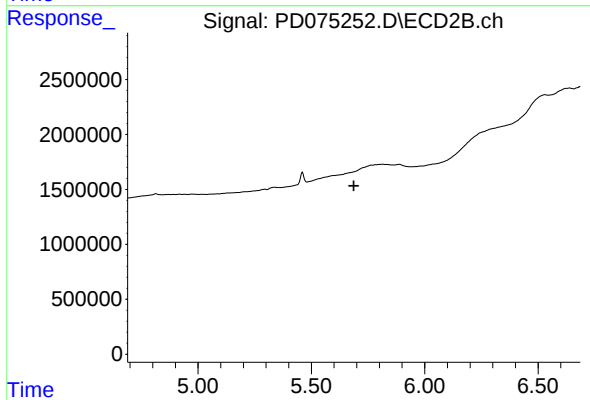


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

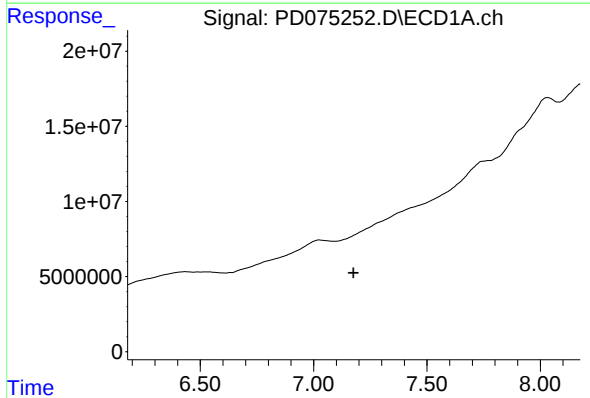


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 7.176 min
Response: 0
Conc: N.D.

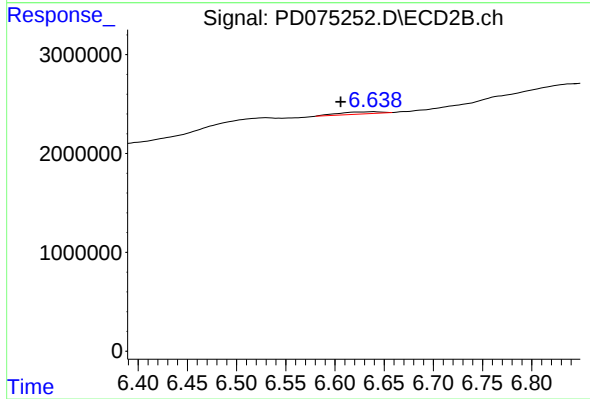

#25 Toxaphene-4


R.T.: 6.640 min
Delta R.T.: 0.034 min
Response: 658505
Conc: 26.01 ng/ml

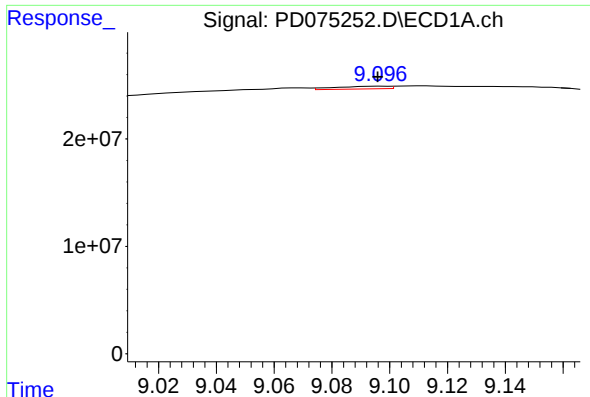

#27 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.002 min
Response: 3253257
Conc: 1.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

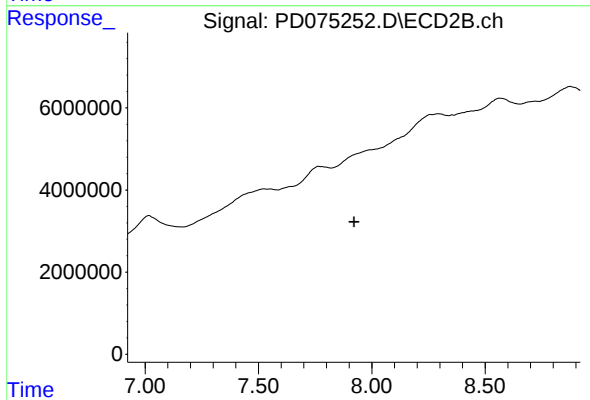

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.922 min
Response: 0
Conc: N.D.