

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
 Data File : PD075215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 16:53
 Operator : AR\AJ
 Sample : PB152520BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS520

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/06/2023
 Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:07:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.771	47607126	21320876	20.872	20.214
27)	SA Decachlor...	9.091	7.918	93367709	34470941	37.729	36.501
Target Compounds							
2)	A alpha-BHC	4.005	3.273	16724604	6670864	4.349	4.307
3)	MA gamma-BHC...	4.339	3.603	15794769	6348886	4.393	4.319
4)	MA Heptachlor	4.930	3.944	17068568	6661232	4.579	4.559
5)	MB Aldrin	5.273	4.223	17196681	7192595	4.715	4.850m
6)	B beta-BHC	4.535	3.900	7605348	3361228	4.633	4.616
7)	B delta-BHC	4.781	4.129	15220736	5986280	4.503m	3.789m
8)	B Heptachlo...	5.695	4.727	47309769	6329434	13.959m	4.538 #
9)	A Endosulfan I	6.088	5.097	14005347	4365729	4.643	3.638
10)	B trans-Chl...	5.957	4.978	13721936	6850587	4.188	5.020
11)	B cis-Chlor...	6.037	5.042	14836362	8386797	4.353	6.010 #
12)	B 4,4'-DDE	6.208	5.231	26609404	11150260	8.148	8.673
13)	MA Dieldrin	6.363	5.363	30026019	12663164	8.780	9.281
14)	MA Endrin	6.592	5.639	25836265	15119038	8.934m	12.430 #
15)	B Endosulfa...	6.813	5.932	26556300	11454967	8.246	8.953
16)	A 4,4'-DDD	6.727	5.786	22267183	9413634	9.214	9.495
17)	MA 4,4'-DDT	7.041	6.038	25108339	8482468	9.892m	8.416
18)	B Endrin al...	6.941	6.112	18570233	8423285	7.850m	8.295
19)	B Endosulfa...	7.178	6.335	22766792	10418561	8.277	8.958
20)	A Methoxychlor	7.516	6.613	57455635	26656205	39.114m	46.538
21)	B Endrin ke...	7.665	6.839	26422300	17370386	8.717	13.173m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
Data File : PD075215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 16:53
Operator : AR\AJ
Sample : PB152520BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:07:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

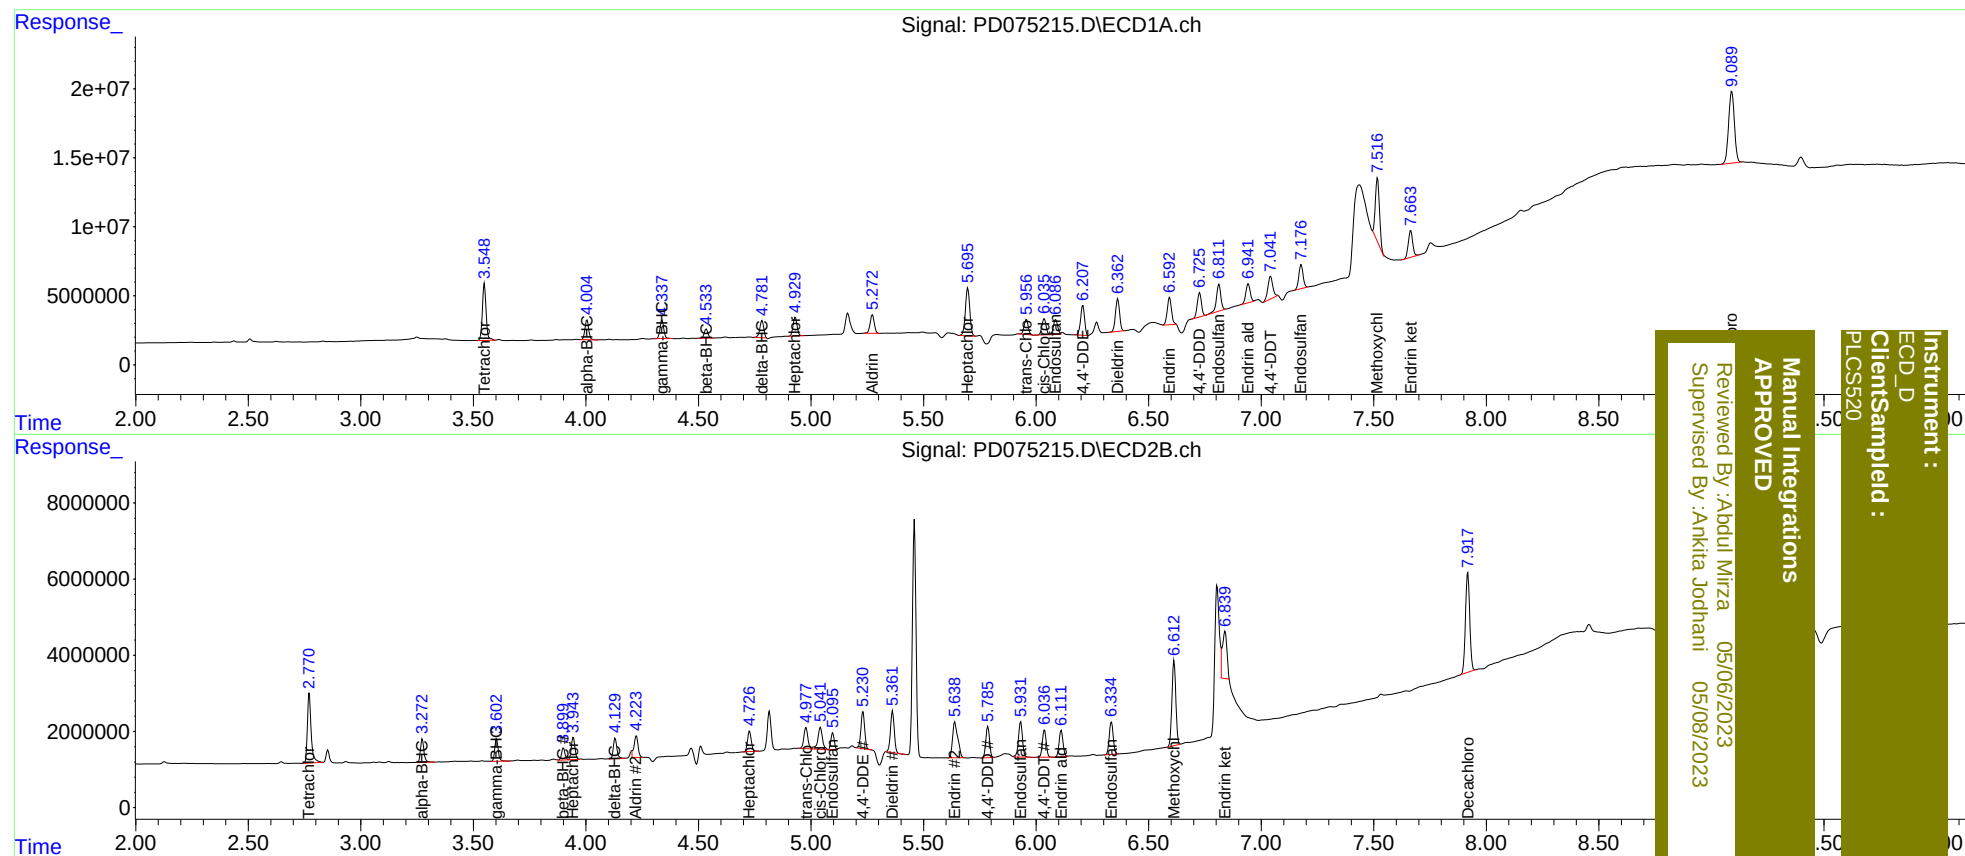

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Instrument :
ECD_D
Client Sampled :
PLCS520