

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
 Data File : PD075218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 19:11
 Operator : AR\AJ
 Sample : 02479-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW944

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/12/2023
 Supervised By : Ankita Jodhani 05/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 00:02:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.773	34712422	10480085	15.219m	9.936 #
2) SA Decachlor...	9.090	7.919	42580601	13711126	17.206m	14.519
Target Compounds						
7) B delta-BHC	4.804	4.142	801.4E6	329.9E6	237.091m	208.799
17) MA 4,4'-DDT	7.015	6.032	742.3E6	315.6E6	292.434m	313.148m
19) B Endosulfa...	7.158	6.333	32914977	22655898	11.966m	19.480m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
Data File : PD075218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 19:11
Operator : AR\AJ
Sample : 02479-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 00:02:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

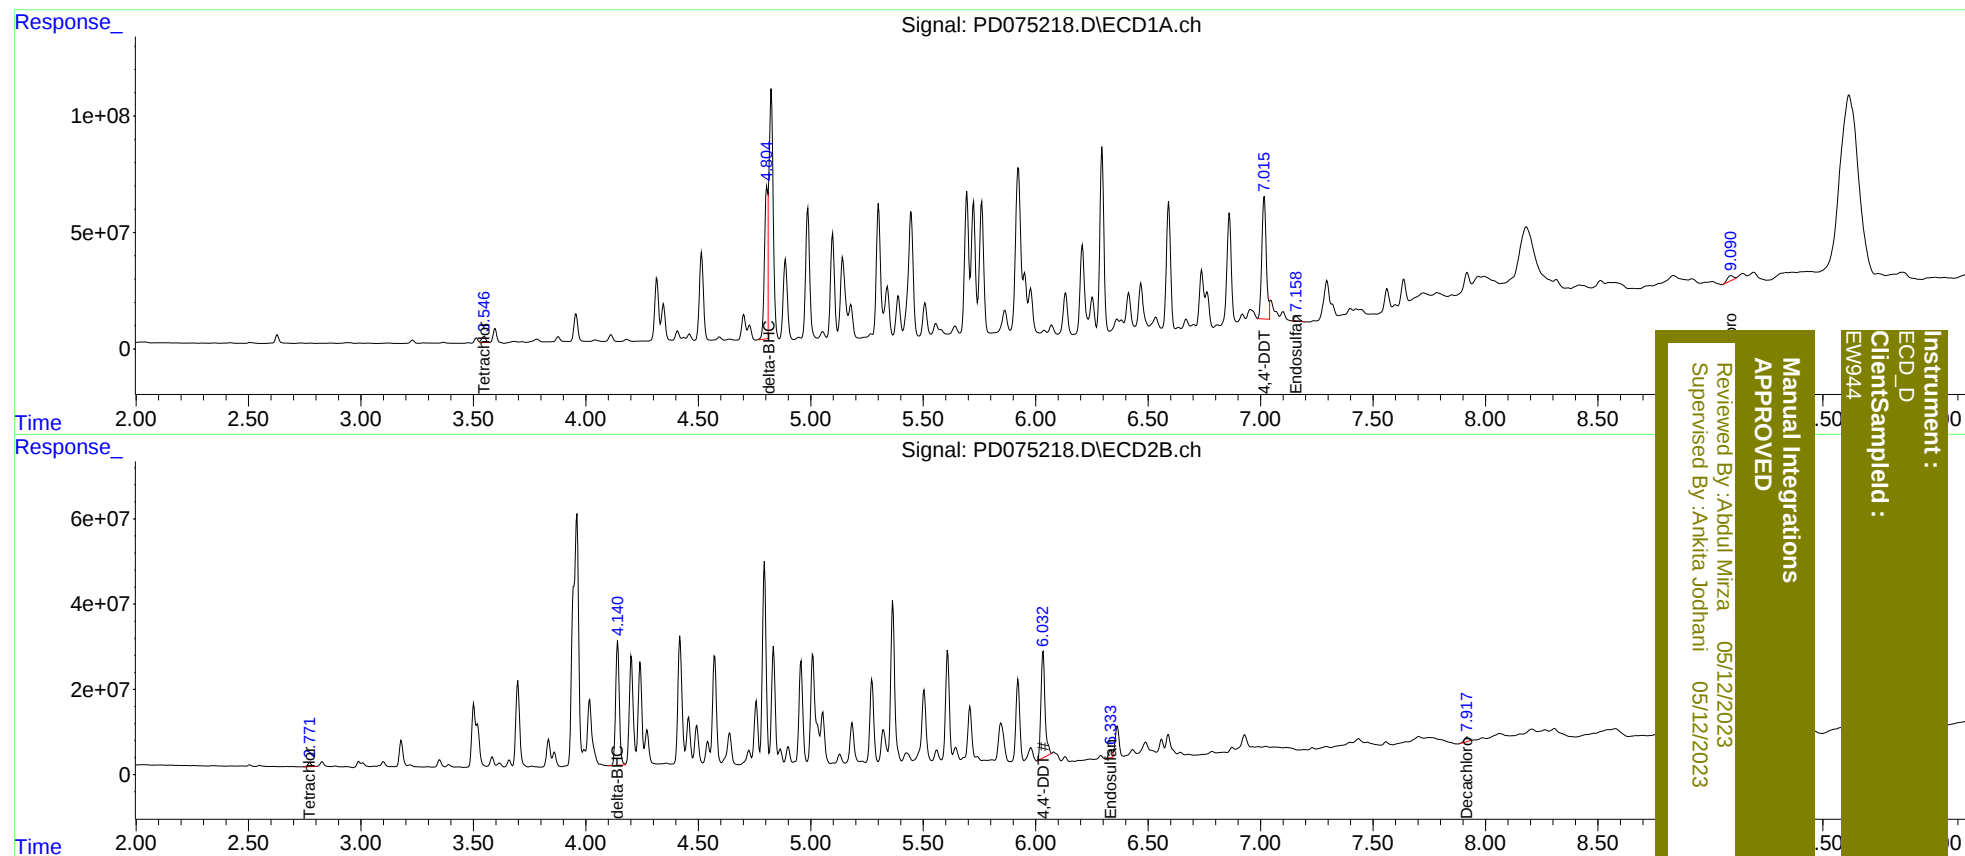

Instrument :
ECD_D
ClientSampled :
EW/944

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/12/2023
Supervised By :Ankita Jodhani 05/12/2023