

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD050423\  
 Data File : PD075224.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 04 May 2023 21:54  
 Operator : AR\AJ  
 Sample : 02479-09  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 EW950

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 05/06/2023  
 Supervised By : Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 04 23:10:05 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD050323CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu May 04 02:14:07 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml    | ng/ml     |
|-----------------------------|-----------------|-------|-------|----------|----------|----------|-----------|
| -----                       |                 |       |       |          |          |          |           |
| System Monitoring Compounds |                 |       |       |          |          |          |           |
| 1)                          | SA Tetrachlo... | 3.548 | 2.772 | 24784809 | 9937726  | 10.866m  | 9.422     |
| 27)                         | SA Decachlor... | 9.092 | 7.918 | 22276885 | 21215986 | 9.002m   | 22.465 #  |
| Target Compounds            |                 |       |       |          |          |          |           |
| 4)                          | MA Heptachlor   | 4.930 | 3.945 | 1366.3E6 | 537.4E6  | 366.500  | 367.801   |
| 8)                          | B Heptachlo...  | 5.700 | 4.727 | 2083.3E6 | 806.2E6  | 614.682  | 578.035   |
| 10)                         | B trans-Chl...  | 5.958 | 4.978 | 2857.0E6 | 1204.3E6 | 871.926  | 882.541   |
| 11)                         | B cis-Chlor...  | 6.038 | 5.042 | 988.9E6  | 285.3E6  | 290.167  | 204.454 # |
| 12)                         | B 4,4'-DDE      | 6.207 | 5.231 | 176.1E6  | 53121167 | 53.922   | 41.321    |
| 13)                         | MA Dieldrin     | 6.363 | 5.363 | 4863.8E6 | 1805.4E6 | 1422.279 | 1323.211  |
| 17)                         | MA 4,4'-DDT     | 7.041 | 6.038 | 226.1E6  | 86061547 | 89.079   | 85.390    |
| -----                       |                 |       |       |          |          |          |           |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD050423\  
Data File : PD075224.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 May 2023 21:54  
Operator : AR\AJ  
Sample : 02479-09  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 04 23:10:05 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD050323CLP.M  
Quant Title : GC Extractables  
QLast Update : Thu May 04 02:14:07 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

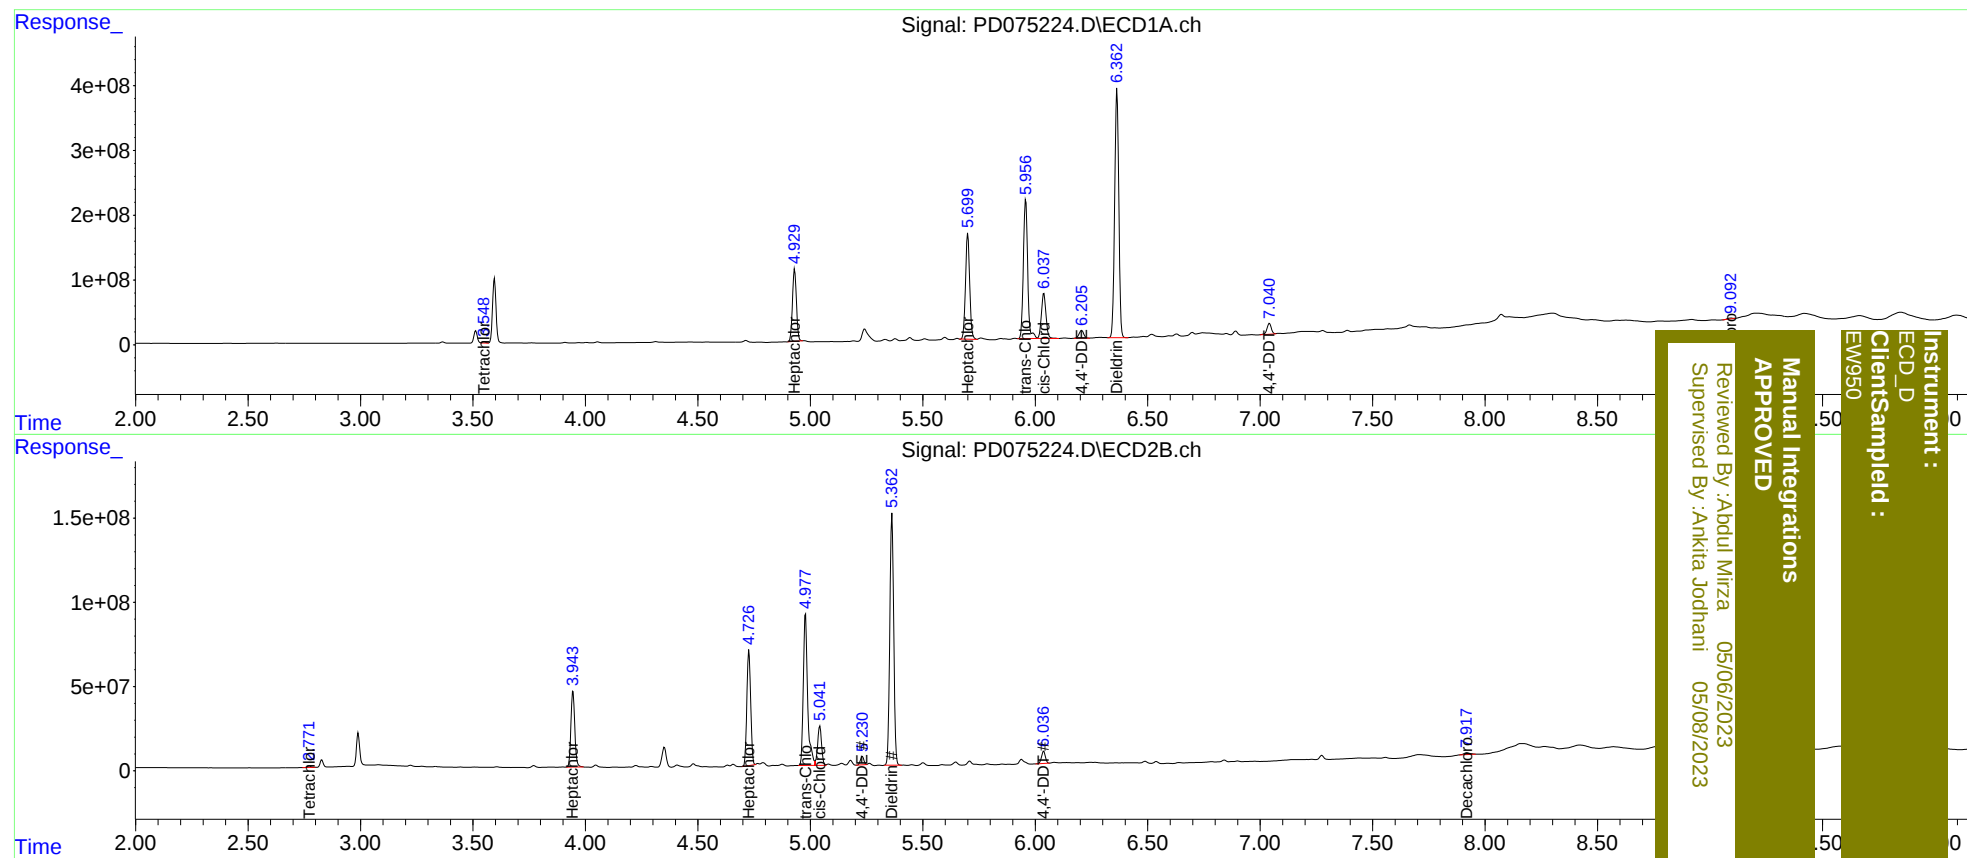

Instrument :  
ECD\_D  
Client Sampled :  
EW/50

Manual Integrations  
APPROVED

Reviewed By : Abdul Mirza 05/06/2023  
Supervised By : Ankita Jodhani 05/08/2023