

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
 Data File : PD075235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 03:32
 Operator : AR\AJ
 Sample : 02479-21MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW975MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/06/2023
 Supervised By : Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 05:02:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.771	26777053	11711761	11.740	11.104
27)	SA Decachlor...	9.084	7.917	24775084	19776502	10.011	20.941 #
Target Compounds							
2)	A alpha-BHC	4.006	3.274	162.9E6	64804385	42.358	41.836
3)	MA gamma-BHC...	4.338	3.605	168.1E6	75849713	46.772m	51.601
4)	MA Heptachlor	4.929	3.943	144.2E6	123.3E6	38.670m	84.410m#
5)	MB Aldrin	5.271	4.225	165.2E6	63125385	45.294m	42.563m
6)	B beta-BHC	4.534	3.899	53249901	25067023	32.440m	34.426m
7)	B delta-BHC	4.785	4.135	104.0E6	102.9E6	30.757m	65.105 #
8)	B Heptachlo...	5.695	4.727	348.5E6	49843186	102.820	35.736 #
9)	A Endosulfan I	6.087	5.099	99825231	34030978	33.094	28.355
10)	B trans-Chl...	5.954	4.976	205.4E6	53643963	62.688m	39.312m#
11)	B cis-Chlor...	6.037	5.041	143.1E6	91987439	41.992	65.913m#
12)	B 4,4'-DDE	6.207	5.231	391.1E6	103.6E6	119.777	80.611 #
13)	MA Dieldrin	6.362	5.364	433.6E6	278.8E6	126.797	204.328 #
14)	MA Endrin	6.592	5.639	449.2E6	117.6E6	155.352	96.695 #
15)	B Endosulfa...	6.811	5.929	168.6E6	161.2E6	52.348	125.974 #
16)	A 4,4'-DDD	6.729	5.786	404.9E6	89114573	167.536	89.889 #
17)	MA 4,4'-DDT	7.039	6.033	308.2E6	224.0E6	121.427m	222.224m#
18)	B Endrin al...	6.941	6.111	170.9E6	68501925	72.241m	67.458m
19)	B Endosulfa...	7.177	6.334	188.8E6	104.5E6	68.632	89.861 #
20)	A Methoxychlor	7.515	6.612	582.7E6	201.3E6	396.708m	351.361m
21)	B Endrin ke...	7.662	6.841	249.0E6	80462045	82.138m	61.020 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
Data File : PD075235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 03:32
Operator : AR\AJ
Sample : 02479-21MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 05:02:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

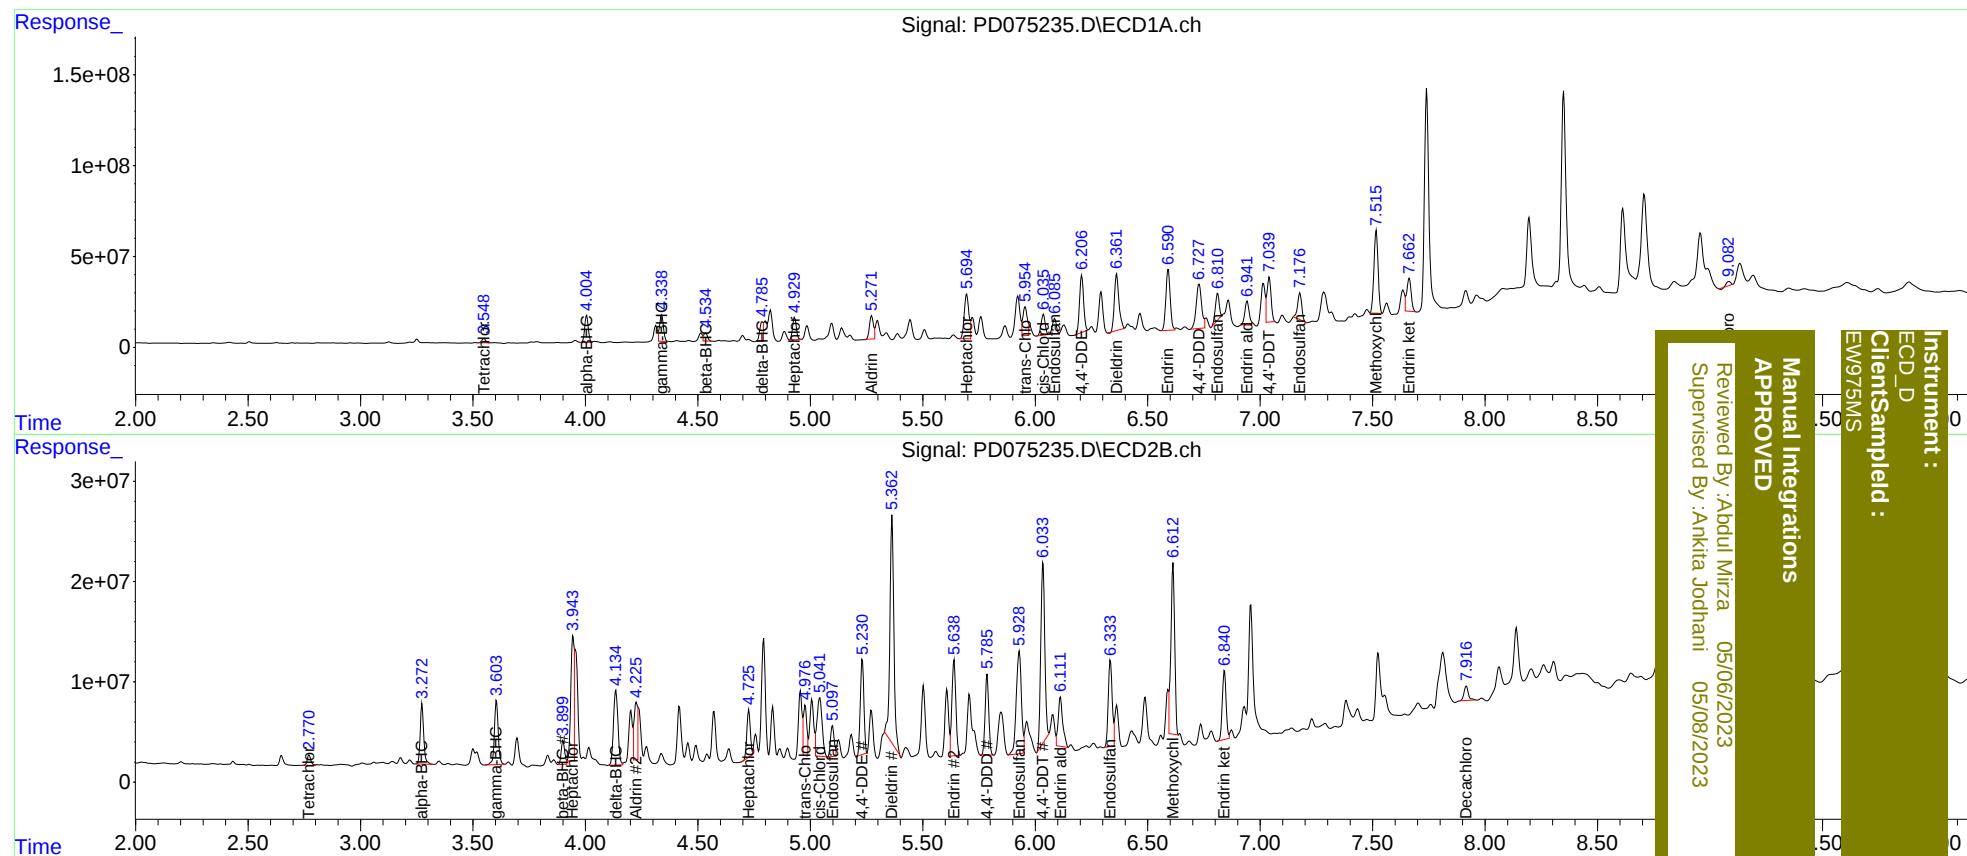

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Instrument :
ECD_D
Client Sampled :
EW/75MS