

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
 Data File : PD075236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 04:00
 Operator : AR\AJ
 Sample : 02479-22MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW975MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/06/2023
 Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 05:02:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.772	25771031	12132830	11.299	11.503
2)	SA Decachlor...	9.083	7.917	41928404	15293723	16.943	16.194
Target Compounds							
2)	A alpha-BHC	4.006	3.274	160.8E6	64355008	41.821	41.546
3)	MA gamma-BHC...	4.338	3.605	168.0E6	75359500	46.725m	51.267
4)	MA Heptachlor	4.929	3.944	141.6E6	99923897	37.977m	68.385m#
5)	MB Aldrin	5.271	4.225	157.1E6	70464258	43.059m	47.512m
6)	B beta-BHC	4.534	3.901	51732440	22834797	31.516m	31.360
7)	B delta-BHC	4.785	4.136	124.9E6	101.5E6	36.963m	64.241 #
8)	B Heptachlo...	5.695	4.727	340.3E6	49885733	100.412	35.766 #
9)	A Endosulfan I	6.086	5.098	96481303	34628277	31.985	28.853
10)	B trans-Chl...	5.954	4.976	236.4E6	53097965	72.142m	38.912m#
11)	B cis-Chlor...	6.036	5.041	140.4E6	87144734	41.186	62.443m#
12)	B 4,4'-DDE	6.208	5.231	384.9E6	102.0E6	117.877	79.370 #
13)	MA Dieldrin	6.362	5.363	428.6E6	268.5E6	125.344	196.789 #
14)	MA Endrin	6.592	5.639	436.2E6	116.4E6	150.830	95.718 #
15)	B Endosulfa...	6.811	5.929	167.7E6	160.8E6	52.061	125.664 #
16)	A 4,4'-DDD	6.729	5.786	397.3E6	89176457	164.412	89.952 #
17)	MA 4,4'-DDT	7.040	6.034	332.4E6	216.9E6	130.972m	215.225 #
18)	B Endrin al...	6.941	6.110	203.4E6	71777518	86.000m	70.684m
19)	B Endosulfa...	7.177	6.334	191.6E6	102.9E6	69.640	88.492 #
20)	A Methoxychlor	7.515	6.611	578.8E6	196.3E6	394.059m	342.661m
21)	B Endrin ke...	7.663	6.841	237.4E6	79045785	78.322	59.946

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
Data File : PD075236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 04:00
Operator : AR\AJ
Sample : 02479-22MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 05:02:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

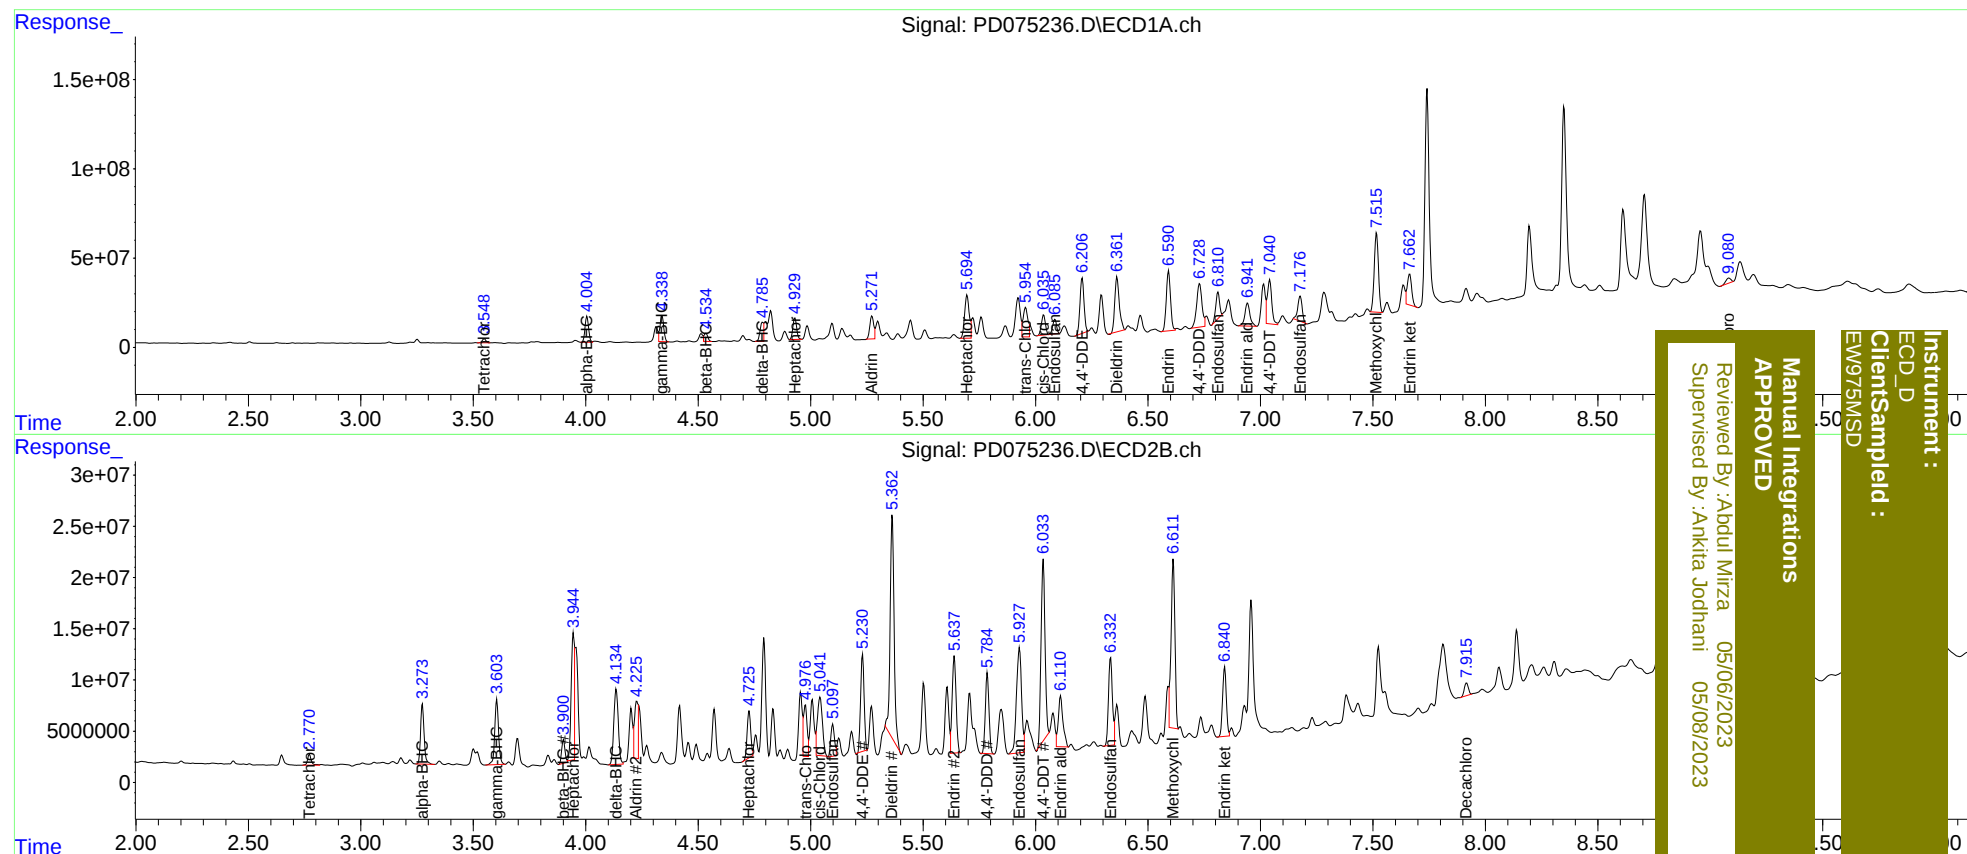

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Instrument :
ECD_D
Client Sampled :
EW/75MSD