

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
 Data File : PD075242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 06:28
 Operator : AR\AJ
 Sample : 02447-13DL 2X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW933DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/12/2023
 Supervised By : Ankita Jodhani 05/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 07:03:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.771	21023754	6571059	9.217	6.230 #
2) SA Decachlor...	9.079	7.914	96435482	30880411	38.968	32.699
Target Compounds						
3) MA gamma-BHC...	4.342	3.611	161.3E6	25630320	44.857m	17.436 #
14) MA Endrin	6.590	5.606	1560.8E6	664.4E6	539.744	546.239m
17) MA 4,4'-DDT	7.013	6.032	1611.8E6	659.1E6	635.006m	653.984
19) B Endosulfa...	7.155	6.330	141.2E6	81068240	51.335m	69.704m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
Data File : PD075242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 06:28
Operator : AR\AJ
Sample : 02447-13DL 2X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 07:03:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

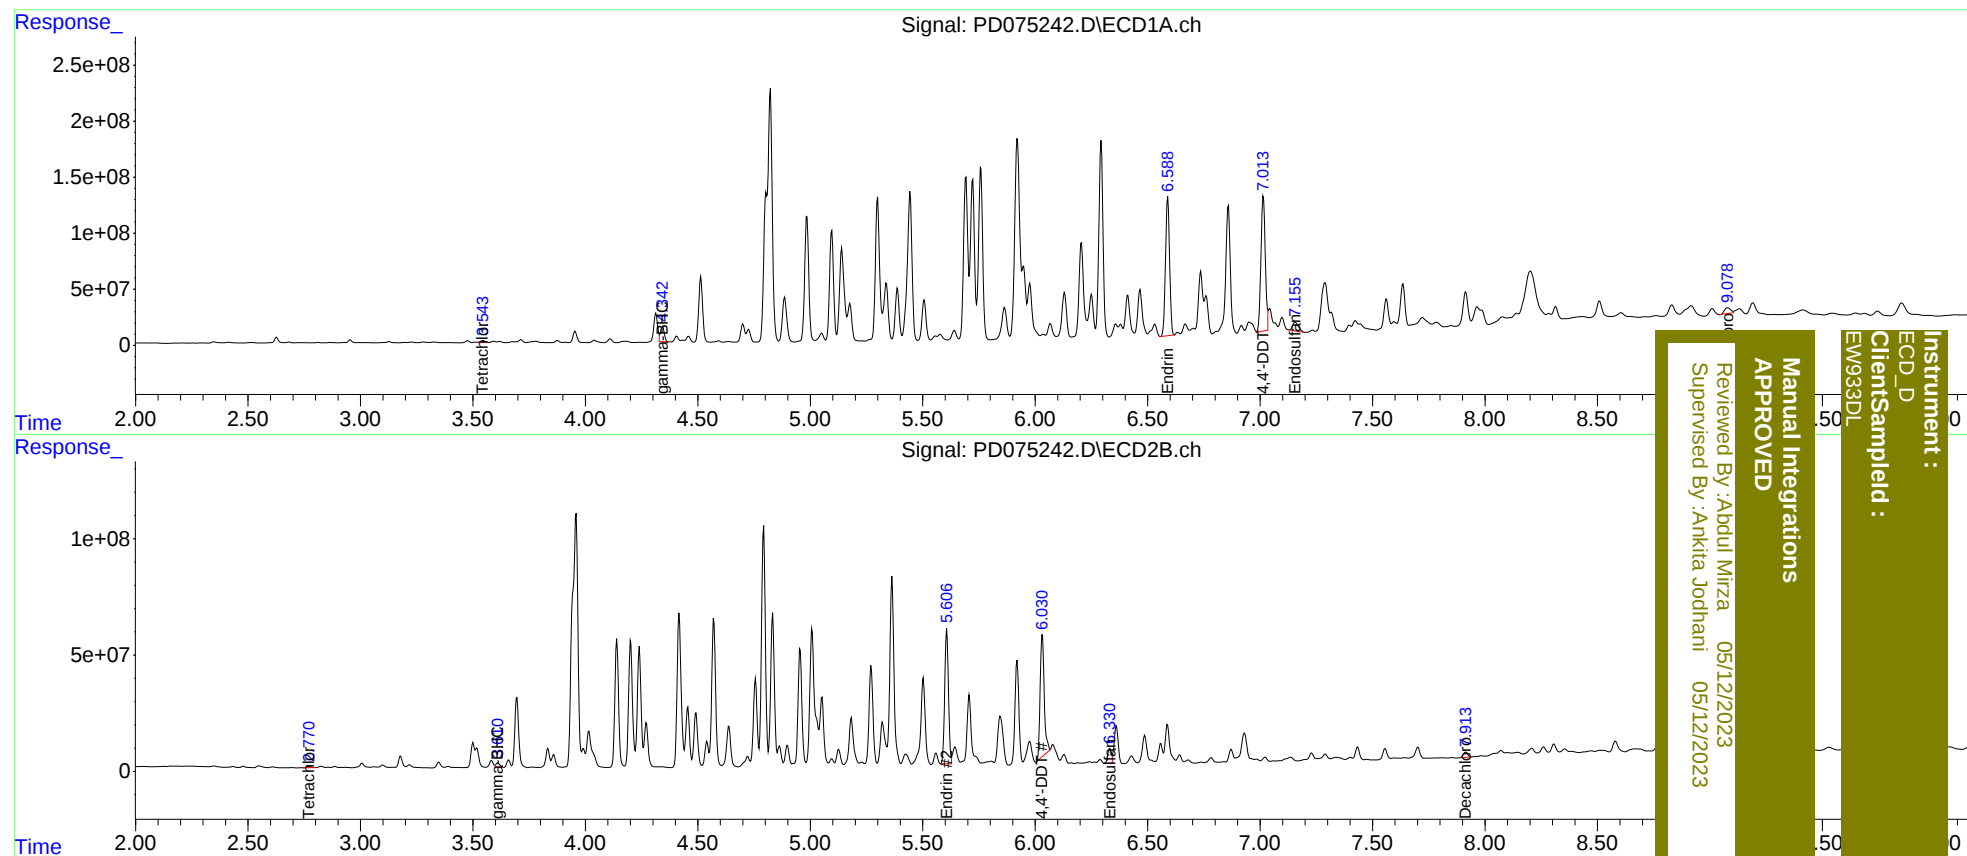

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/12/2023
Supervised By: Ankita Jodhani 05/12/2023

Instrument :
ECD_D
Client Sampled :
EW/933DL