

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
 Data File : PD075246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 07:22
 Operator : AR\AJ
 Sample : 02447-15DL 4X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW935DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/11/2023
 Supervised By :Ankita Jodhani 05/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 08:22:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.771	10845503	3398348	4.755	3.222 #
2) SA Decachlor...	9.085	7.916	23026676	9232114	9.305	9.776
Target Compounds						
7) B delta-BHC	4.802	4.141	851.5E6	354.6E6	251.924m	224.416
14) MA Endrin	6.590	5.606	987.6E6	437.5E6	341.526	359.722m
17) MA 4,4'-DDT	7.013	6.032	1037.4E6	472.8E6	408.700m	469.105
19) B Endosulfa...	7.155	6.330	49006851	32323893	17.816m	27.793m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
Data File : PD075246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 07:22
Operator : AR\AJ
Sample : 02447-15DL 4X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 08:22:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

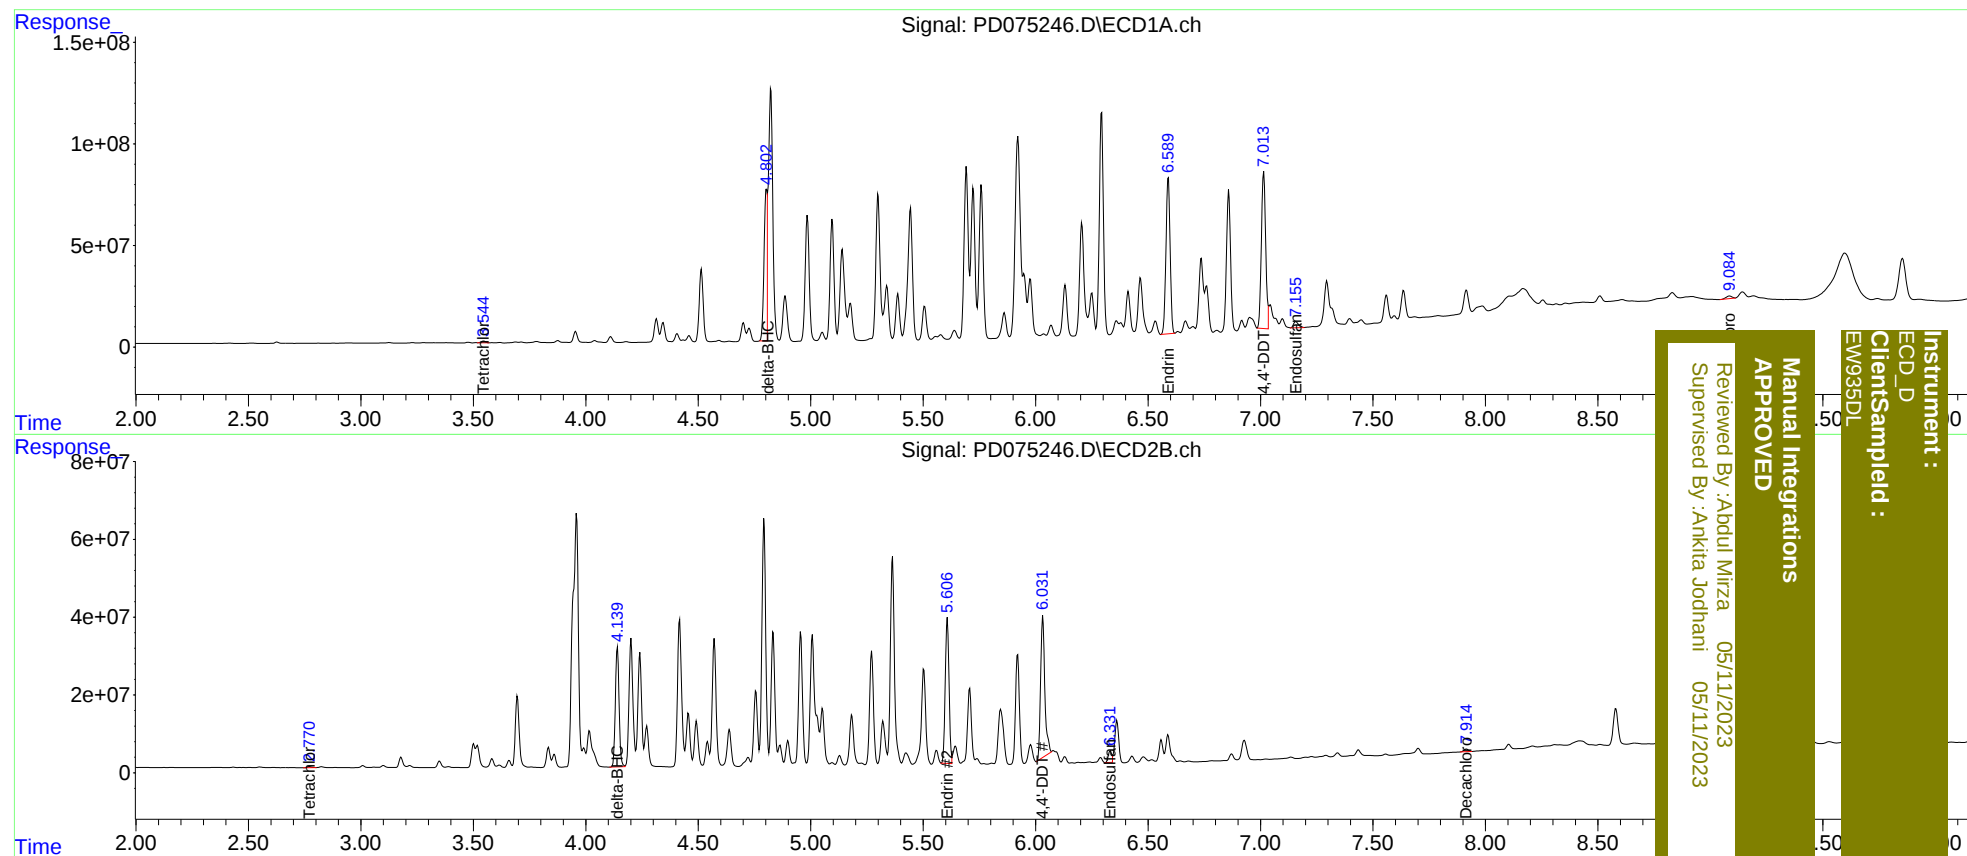

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 05/11/2023
Supervised By: Ankita Jodhani 05/11/2023

Instrument :
ECD_D
Client Sampled :
EW/935DL