

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
 Data File : PD075219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2023 19:38
 Operator : AR\AJ
 Sample : 02479-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW945

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/06/2023
 Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 01:38:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.772	18844868	12650759	8.262m	11.994 #
27)	SA Decachlor...	9.081	7.916	208.5E6	31305848	84.248	33.149m#
Target Compounds							
9)	A Endosulfan I	6.122	5.125	209.1E6	239.2E6	69.327m	199.335m#
12)	B 4,4'-DDE	6.207	5.243	27485494	16259584	8.417m	12.648m#
14)	MA Endrin	6.590	5.637	76594212	18127218	26.487m	14.903m#
16)	A 4,4'-DDD	6.724	5.785	45917952	10703652	19.001m	10.797m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050423\
Data File : PD075219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2023 19:38
Operator : AR\AJ
Sample : 02479-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:38:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

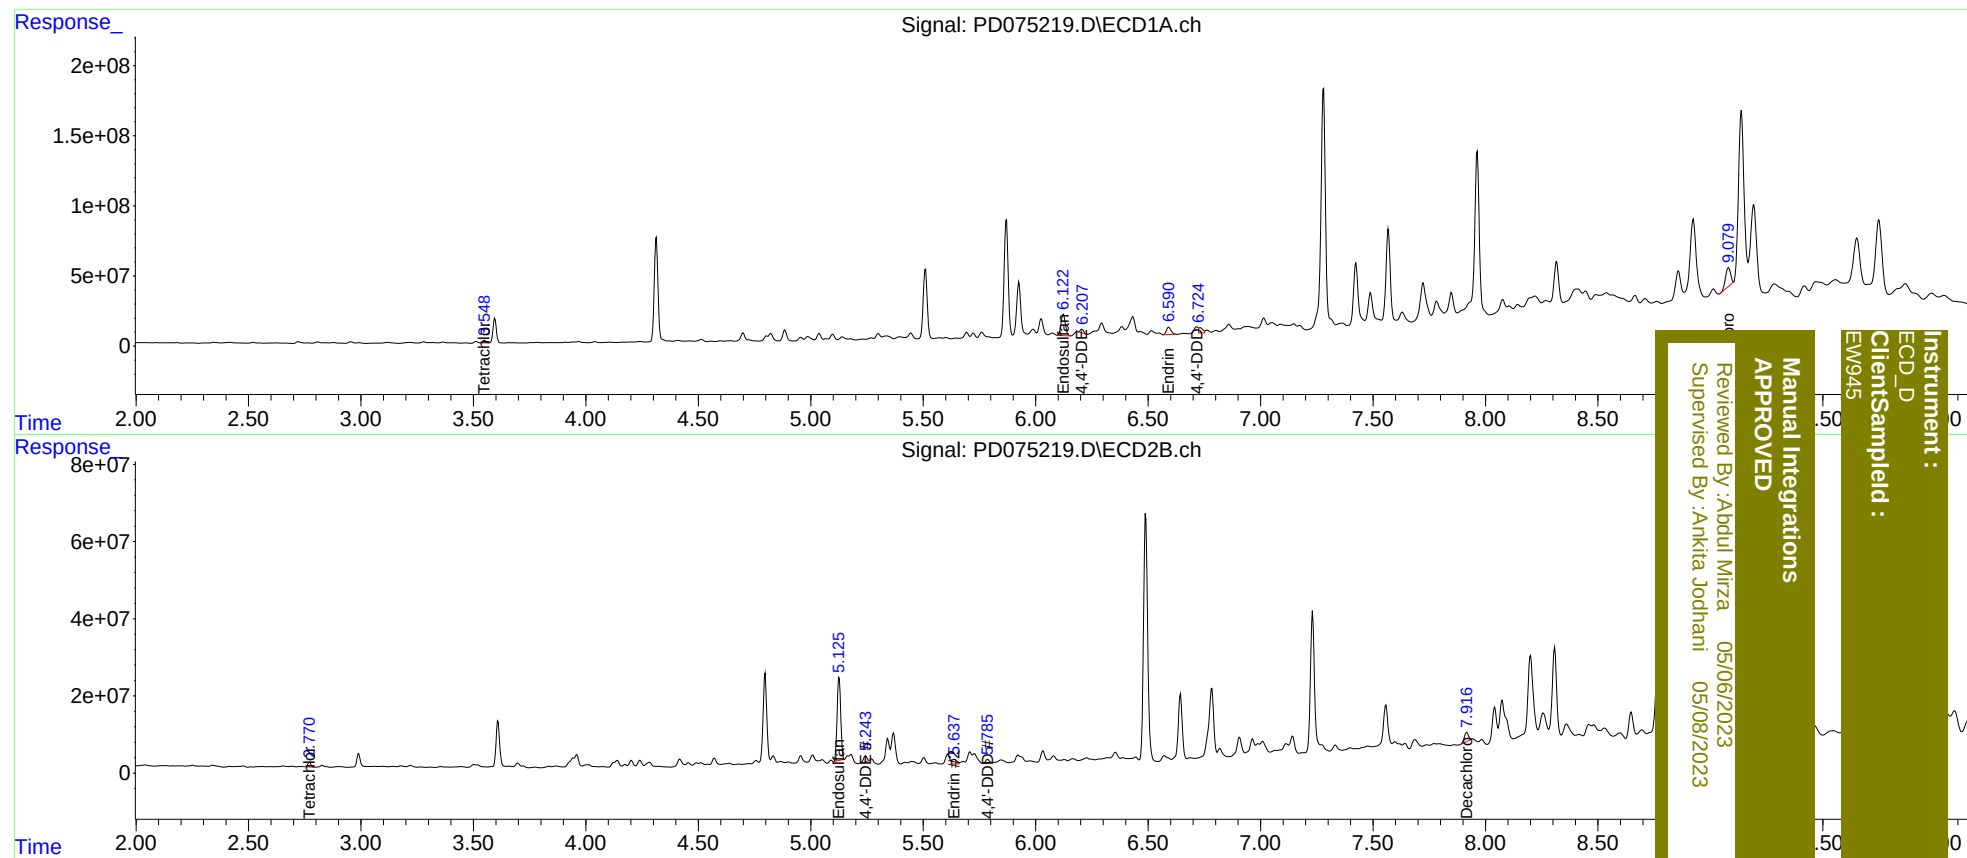

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Instrument :
ECD_D
Client Sampled :
EW/945