

Data Path : P:\HPCHEM1\ECD_D\Data\PD050518\
 Data File : PD047433.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2018 18:29
 Operator : UA/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 05 00:23:55 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD050518.M
 Quant Title : GC Extractables
 QLast Update : Fri May 04 23:48:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.041	21908602	374.3E6	19.282	20.114
28)	SA Decachlor...	8.148	9.120	25011029	409.8E6	19.485	20.476
Target Compounds							
2)	A alpha-BHC	0.000	4.428	0	20274151	N.D.	0.658 #
6)	B beta-BHC	4.355f	4.918f	841314	2697768	1.145	0.222 #
7)	B delta-BHC	0.000	5.080	0	19525960	N.D.	0.673 #
14)	MA Endrin	0.000	6.811f	0	5668444	N.D.	0.274 #
15)	B Endosulfa...	6.165f	0.000	6569	0	0.005	N.D. #
16)	A 4,4'-DDD	0.000	6.811f	0	5668444	N.D.	0.285 #
20)	A Methoxychlor	6.832f	0.000	2993734	0	4.008	N.D. #
23)	Chlordane-1	4.314	5.080	325467	19525960	5.674	18.848 #
27)	Chlordane-5	6.165	0.000	6569	0	0.112	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_D\Data\PD050518\
Data File : PD047433.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2018 18:29
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 05 00:23:55 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD050518.M
Quant Title : GC Extractables
QLast Update : Fri May 04 23:48:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

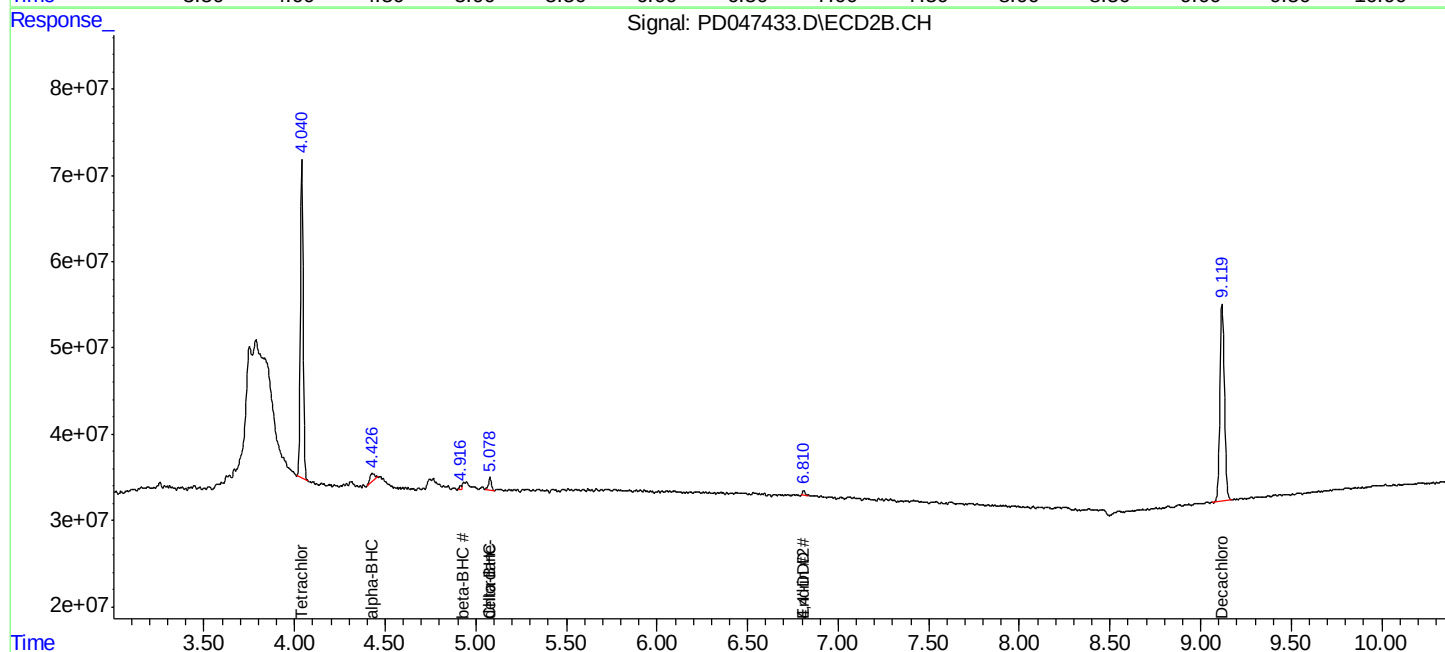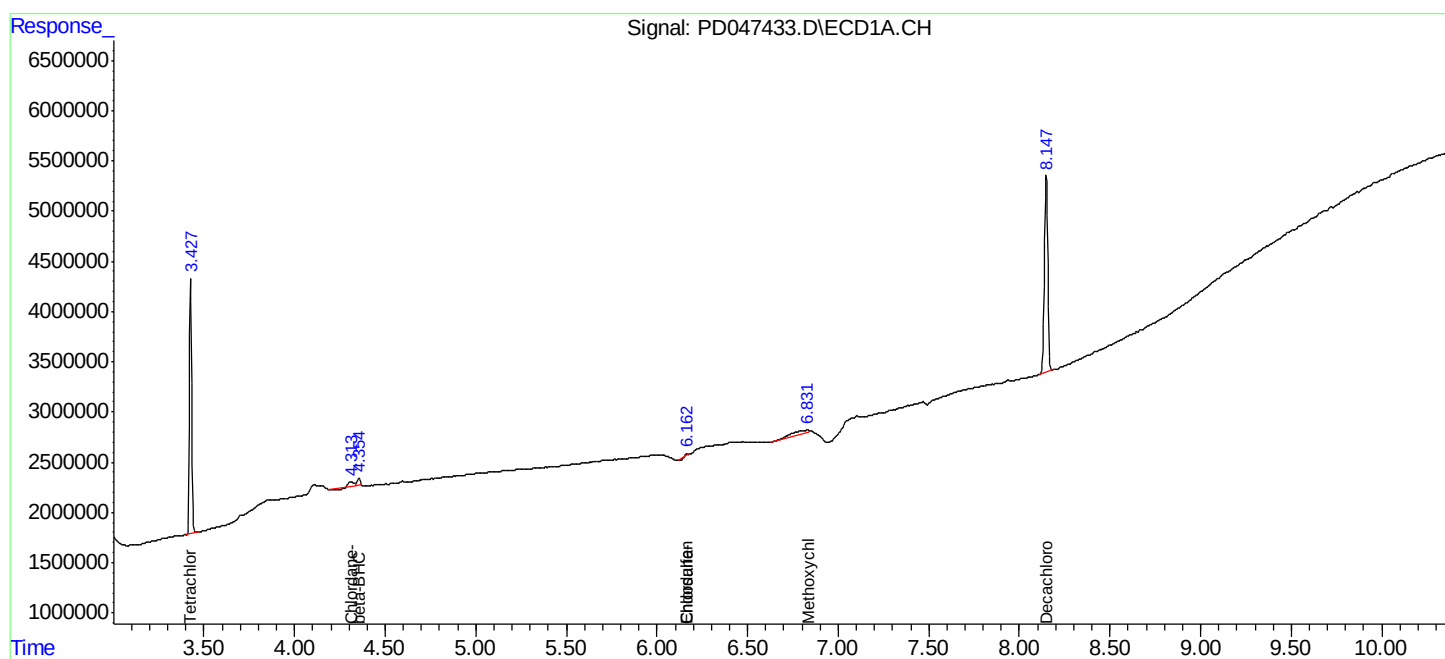


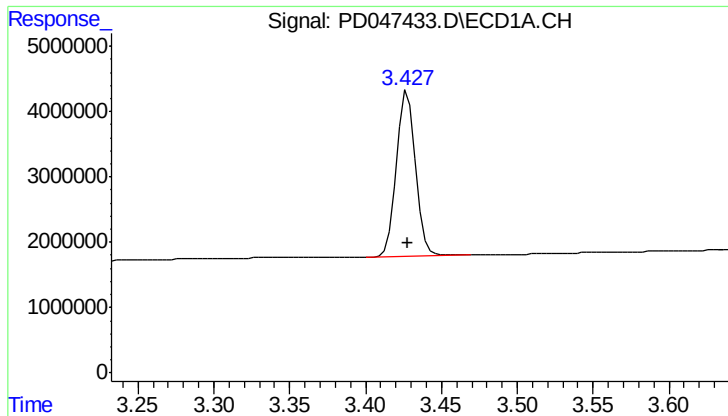

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 21908602
Conc: 19.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

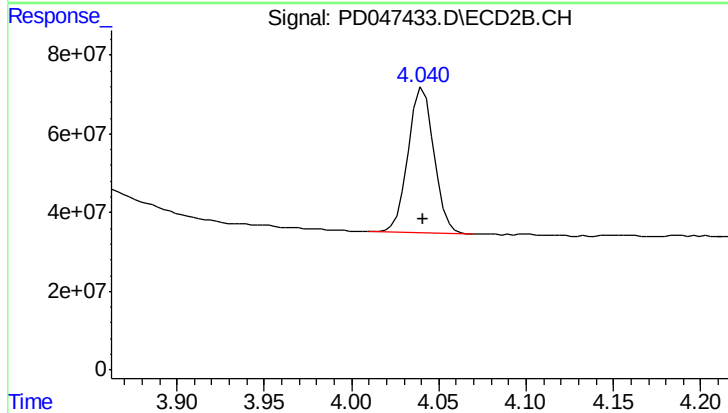


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: 0.000 min
Response: 374339654
Conc: 20.11 ng/ml

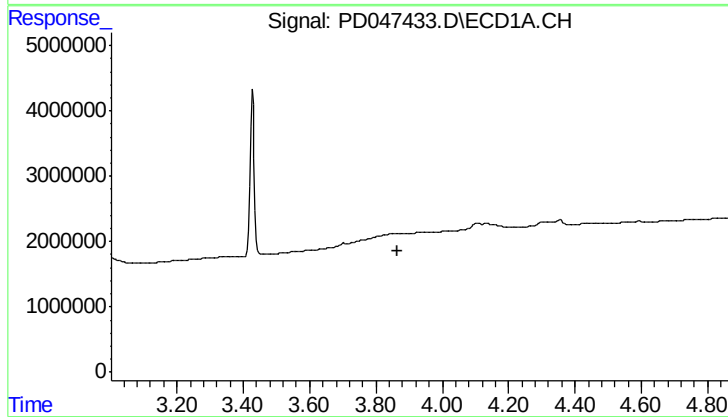


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 3.865 min
Response: 0
Conc: N.D.

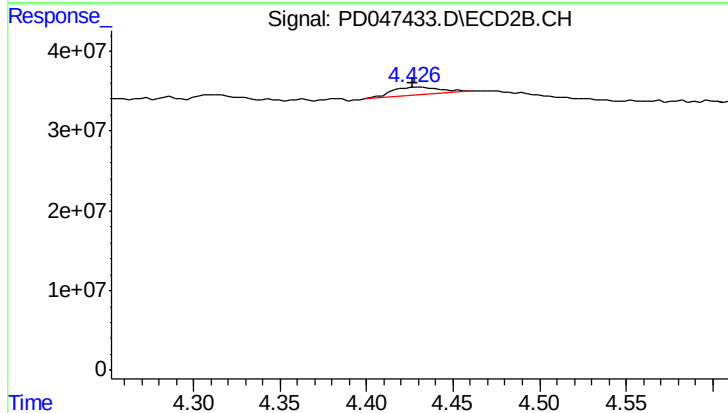

#2 alpha-BHC


R.T.: 4.428 min
Delta R.T.: 0.002 min
Response: 20274151
Conc: 0.66 ng/ml

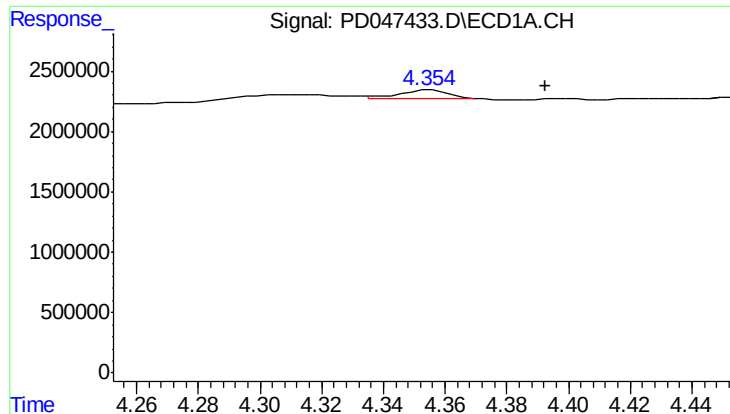

#6 beta-BHC


R.T.: 4.355 min
Delta R.T.: -0.037 min
Response: 841314
Conc: 1.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

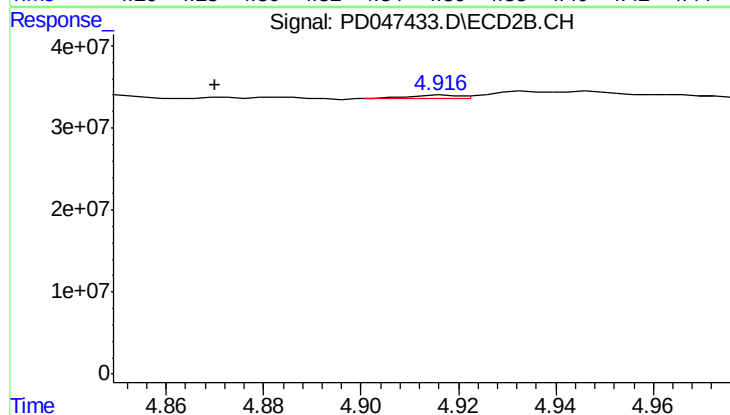


#6 beta-BHC

R.T.: 4.918 min
Delta R.T.: 0.048 min
Response: 2697768
Conc: 0.22 ng/ml

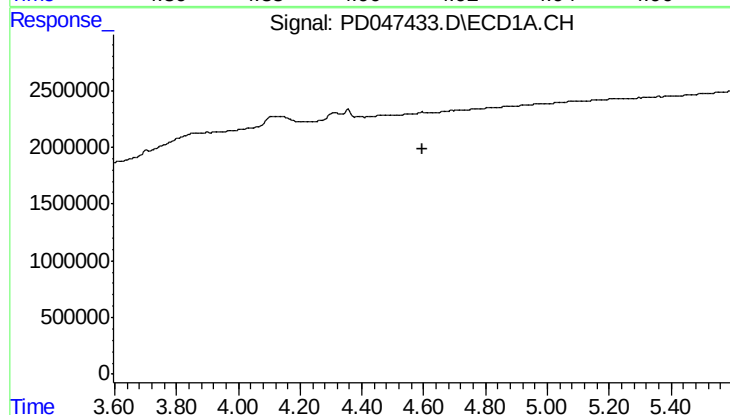


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.594 min
Response: 0
Conc: N.D.

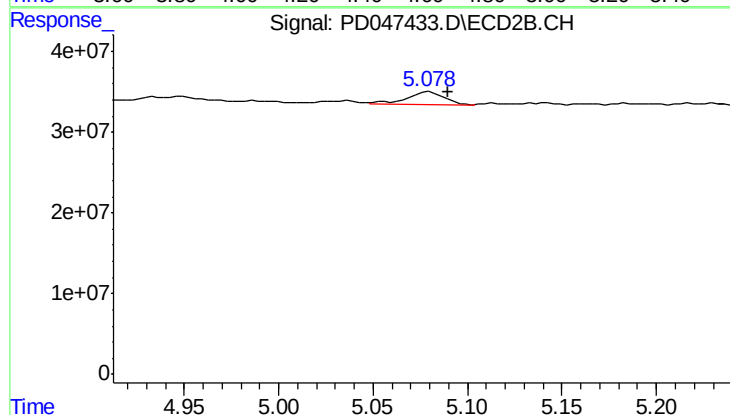

#7 delta-BHC


R.T.: 5.080 min
Delta R.T.: -0.010 min
Response: 19525960
Conc: 0.67 ng/ml

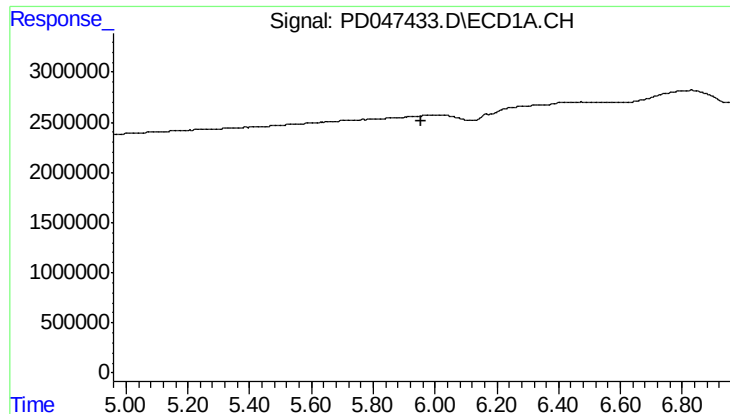

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

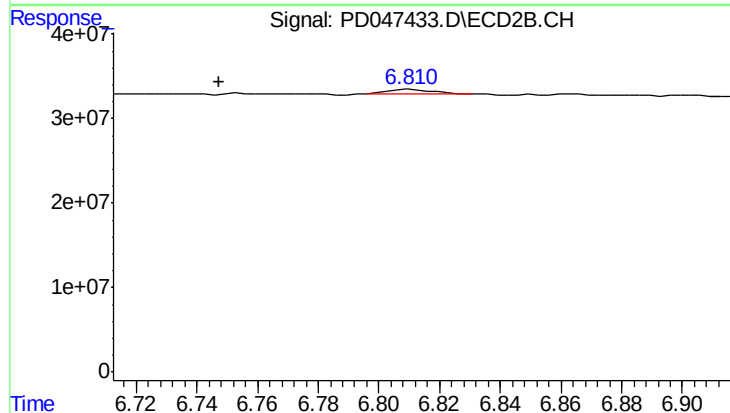


#14 Endrin

R.T.: 6.811 min
Delta R.T.: 0.063 min
Response: 5668444
Conc: 0.27 ng/ml

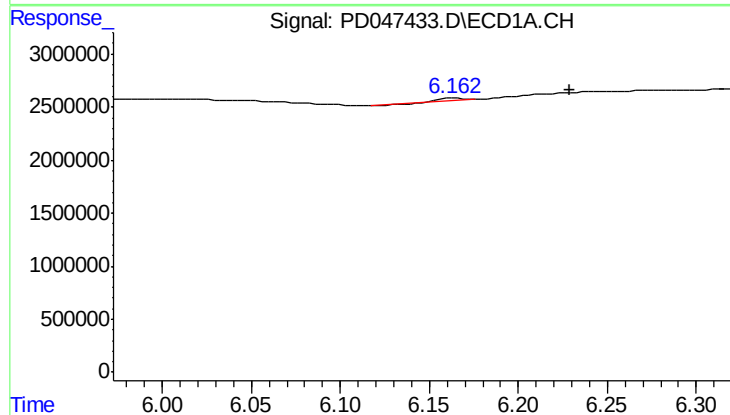


#15 Endosulfan II

R.T.: 6.165 min
Delta R.T.: -0.065 min
Response: 6569
Conc: 0.00 ng/ml

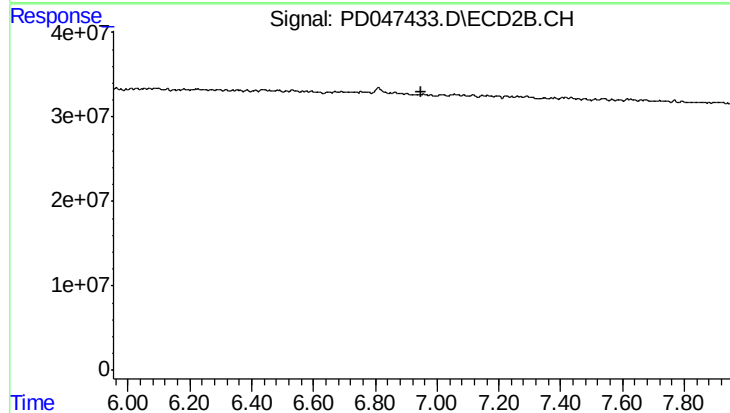

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.949 min
Response: 0
Conc: N.D.

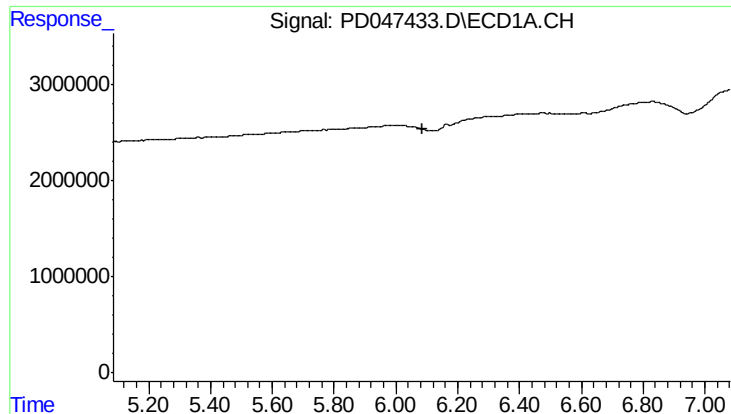

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

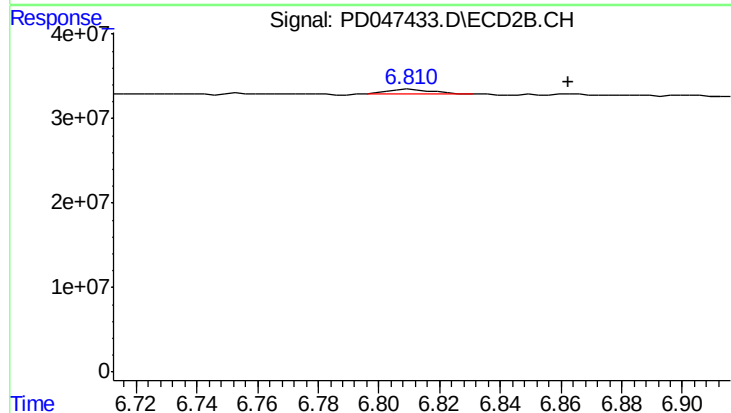


#16 4,4'-DDD

R.T.: 6.811 min
Delta R.T.: -0.052 min
Response: 5668444
Conc: 0.28 ng/ml

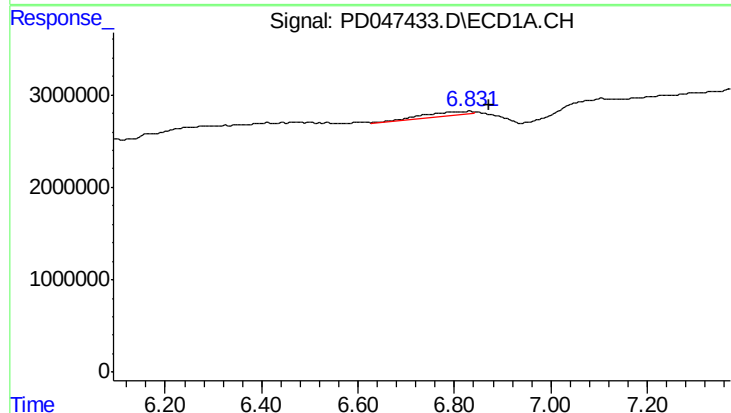


#20 Methoxychlor

R.T.: 6.832 min
Delta R.T.: -0.040 min
Response: 2993734
Conc: 4.01 ng/ml

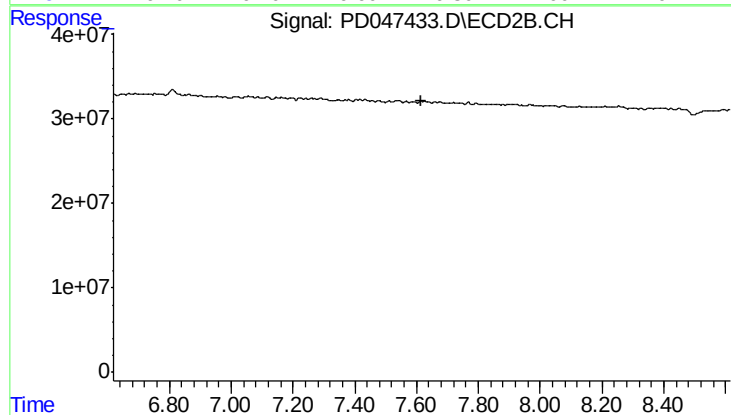

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.616 min
Response: 0
Conc: N.D.

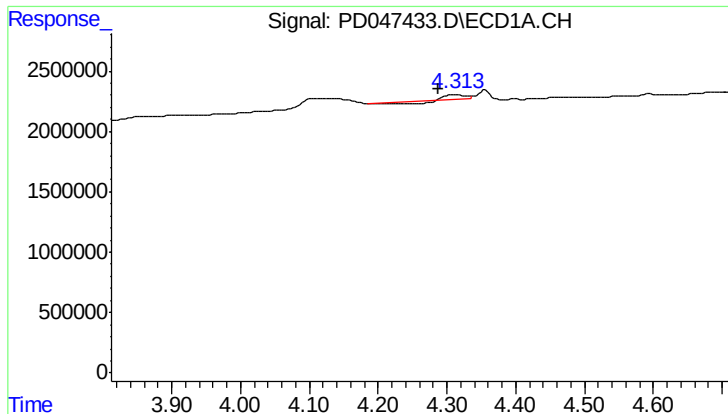

#23 Chlordane-1


R.T.: 4.314 min
Delta R.T.: 0.026 min
Response: 325467
Conc: 5.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

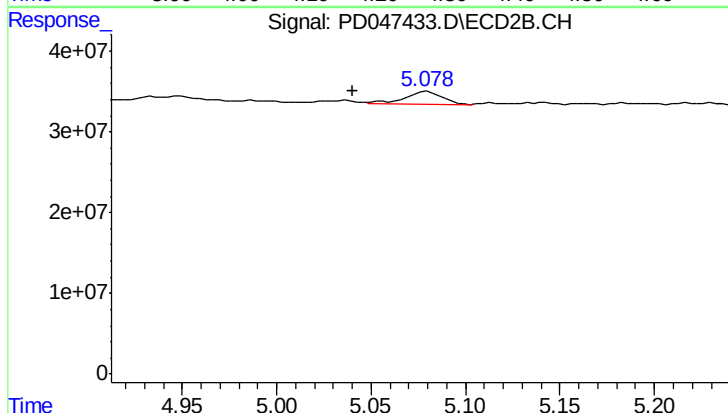


#23 Chlordane-1

R.T.: 5.080 min
Delta R.T.: 0.040 min
Response: 19525960
Conc: 18.85 ng/ml

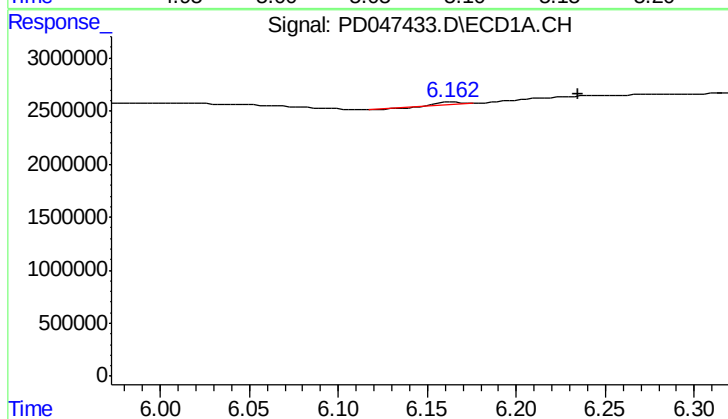


#27 Chlordane-5

R.T.: 6.165 min
Delta R.T.: -0.070 min
Response: 6569
Conc: 0.11 ng/ml

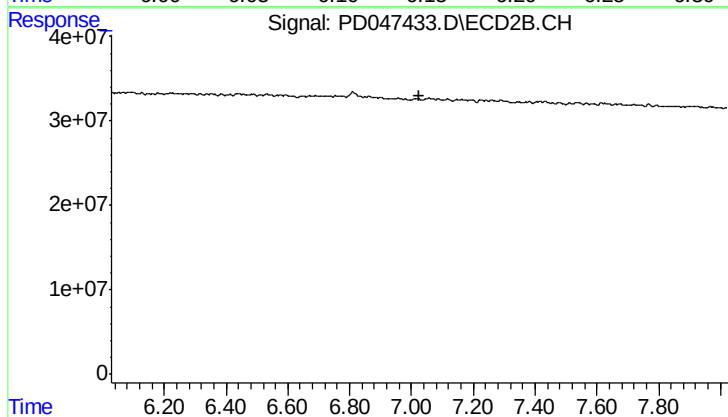

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.027 min
Response: 0
Conc: N.D.

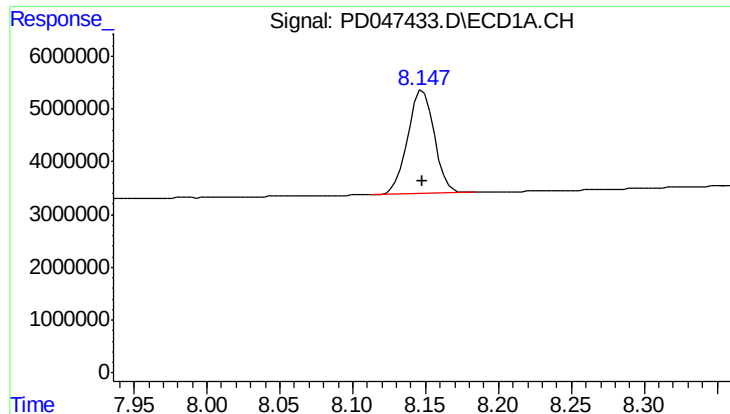

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 25011029
Conc: 19.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

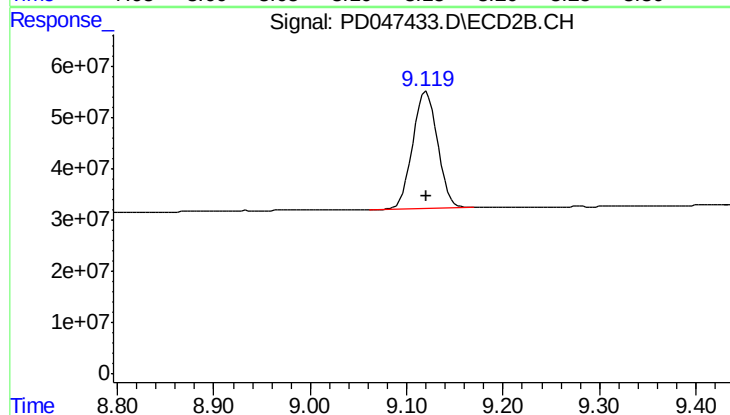

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 409768994
Conc: 20.48 ng/ml