

Data Path : P:\HPCHEM1\ECD_D\Data\PD050518\
 Data File : PD047452.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2018 23:12
 Operator : UA/AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICPD050518CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:58:22 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD050518.M
 Quant Title : GC Extractables
 QLast Update : Fri May 04 23:45:47 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.041	62770831	912.5E6	50.303	49.466
28)	SA Decachlor...	8.147	9.120	64317731	958.1E6	49.557	48.032
Target Compounds							
23)	Chlordane-1	4.288	5.041	27943866	511.3E6	487.189	493.540
24)	Chlordane-2	4.784	5.507	28388623	481.2E6	506.952	466.777
25)	Chlordane-3	5.346	6.152	89323013	1663.3E6	526.542	491.898
26)	Chlordane-4	5.404	6.228	76831494	1904.4E6	506.798	489.854
27)	Chlordane-5	6.236	7.028	30150579	418.4E6	514.000	500.208



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_D\Data\PD050518\
Data File : PD047452.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2018 23:12
Operator : UA/AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD050518CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:58:22 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD050518.M
Quant Title : GC Extractables
QLast Update : Fri May 04 23:45:47 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

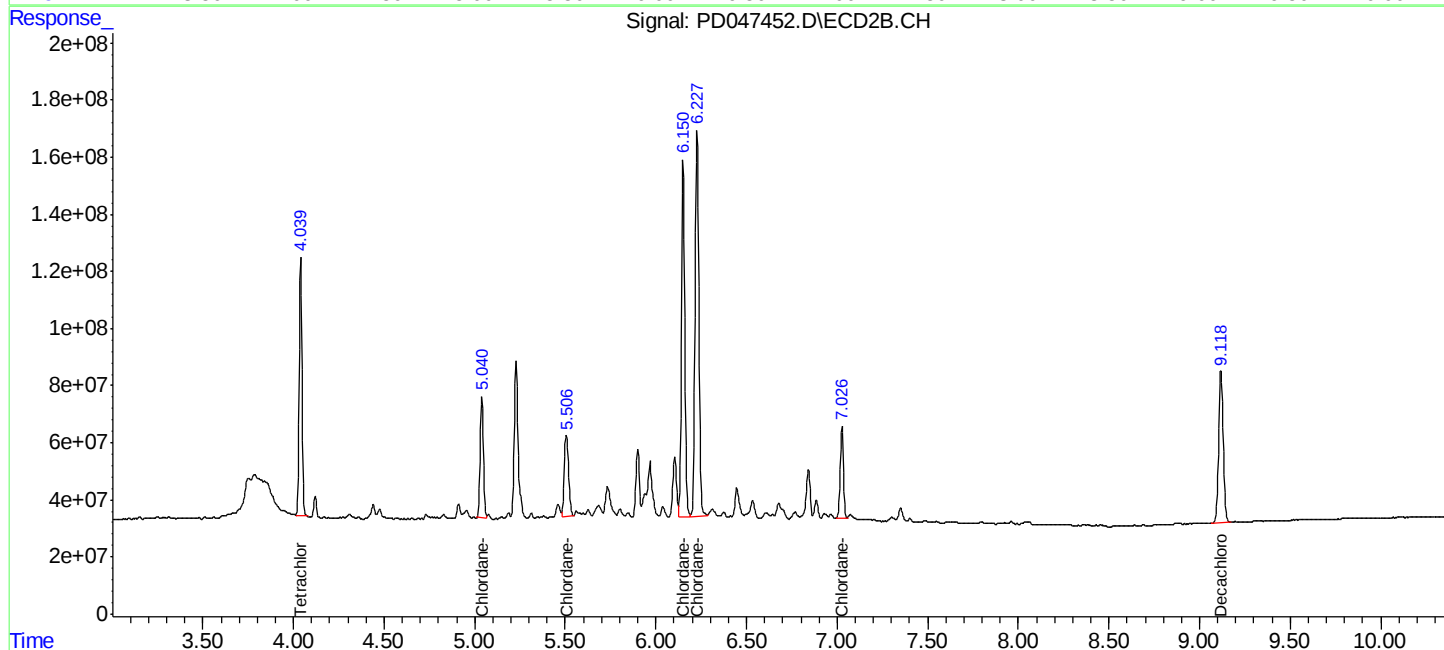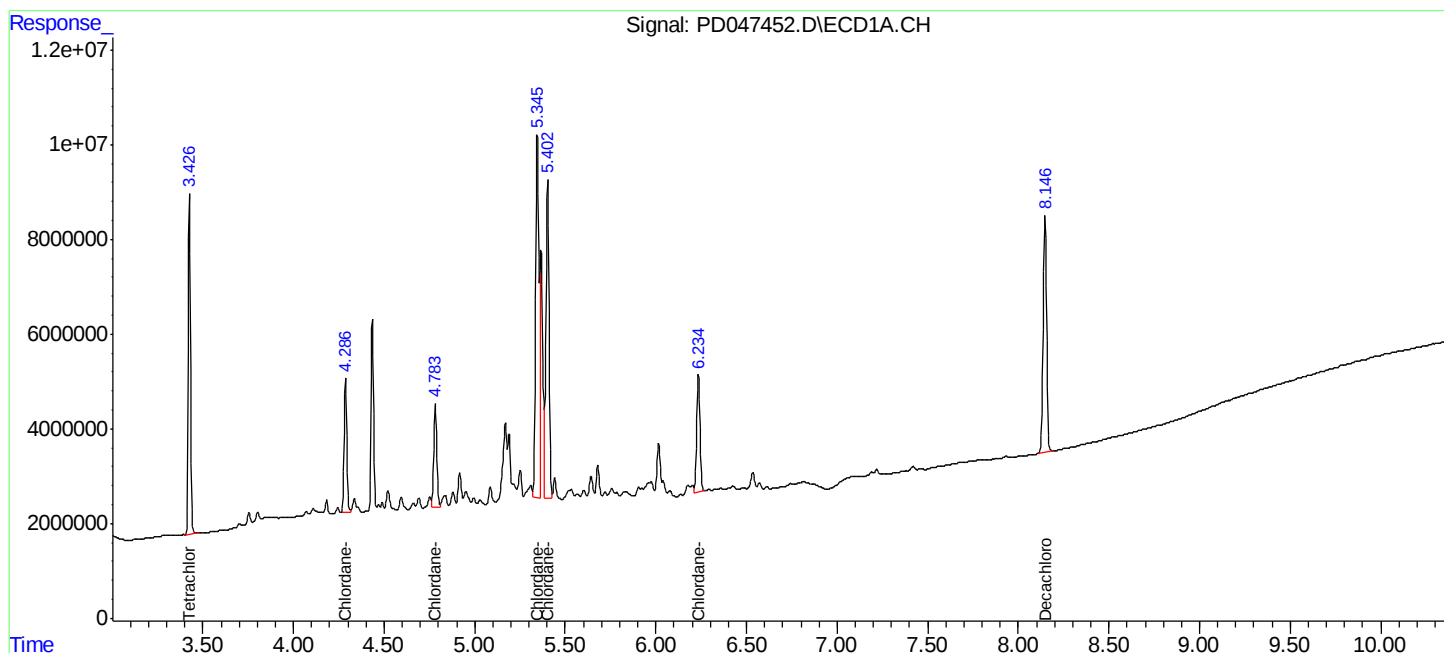


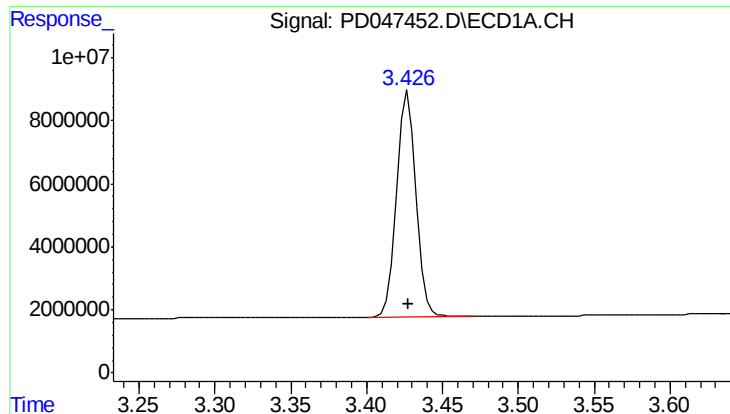

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 62770831
Conc: 50.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD050518CHLOR

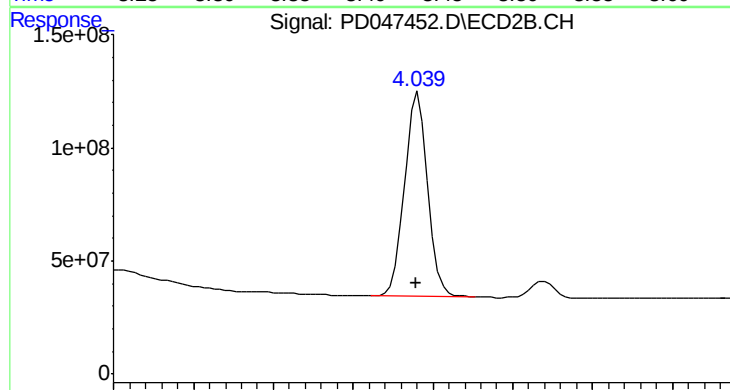


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: 0.002 min
Response: 912547645
Conc: 49.47 ng/ml

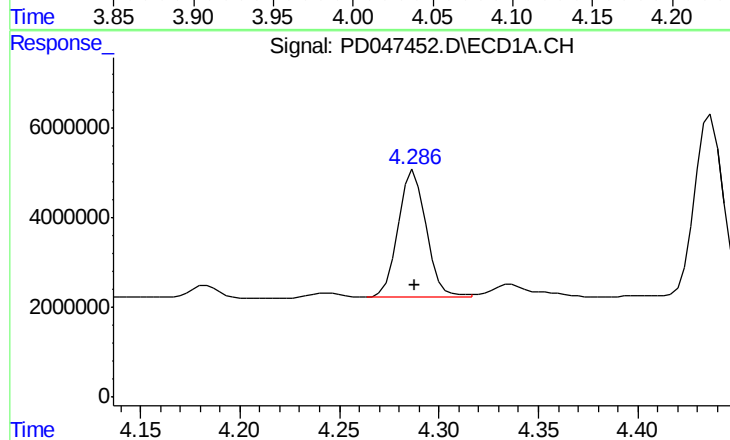


#23 Chlordane-1

R.T.: 4.288 min
Delta R.T.: 0.000 min
Response: 27943866
Conc: 487.19 ng/ml

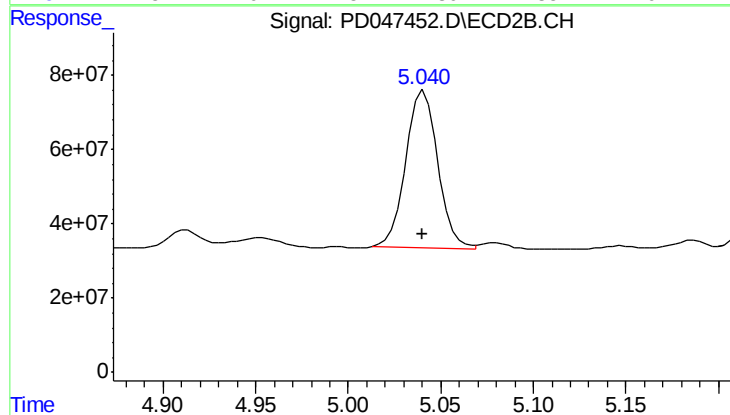

#23 Chlordane-1


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 511303527
Conc: 493.54 ng/ml

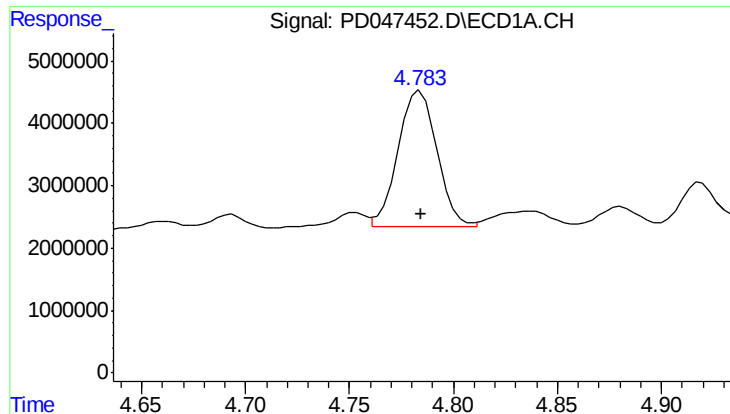

#24 Chlordane-2


R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 28388623
Conc: 506.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD050518CHLOR

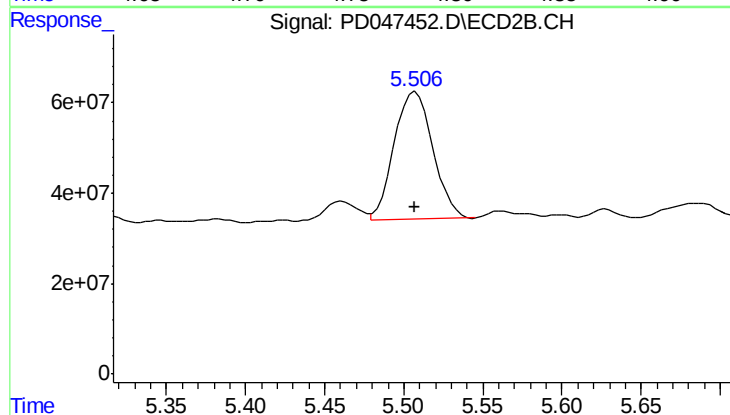


#24 Chlordane-2

R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 481182521
Conc: 466.78 ng/ml

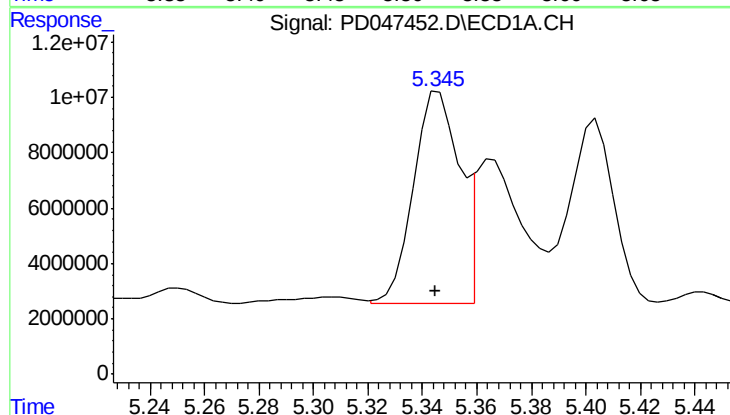


#25 Chlordane-3

R.T.: 5.346 min
Delta R.T.: 0.002 min
Response: 89323013
Conc: 526.54 ng/ml

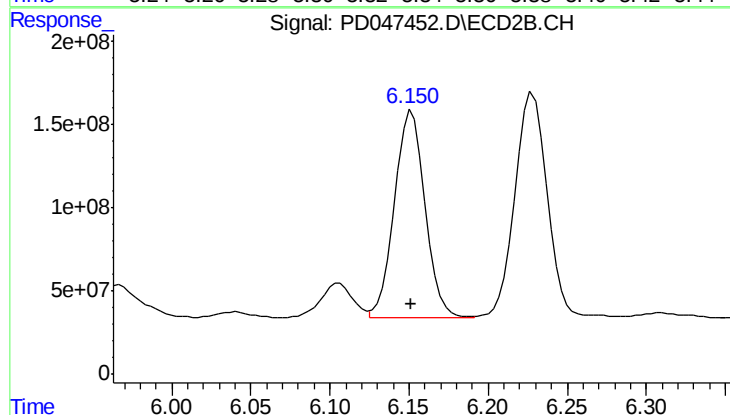

#25 Chlordane-3


R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 1663257242
Conc: 491.90 ng/ml

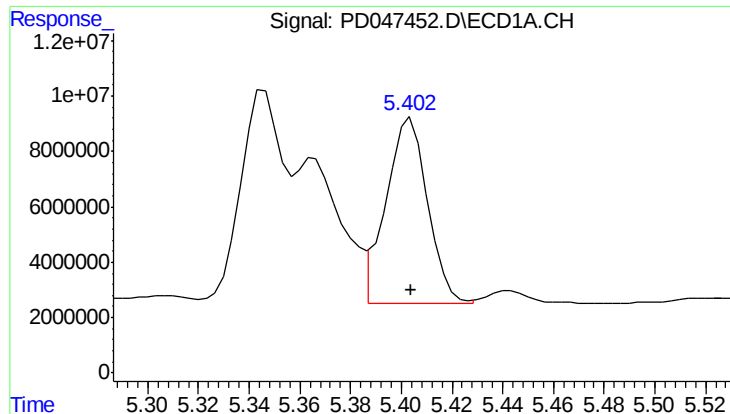

#26 Chlordane-4


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 76831494
Conc: 506.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD050518CHLOR

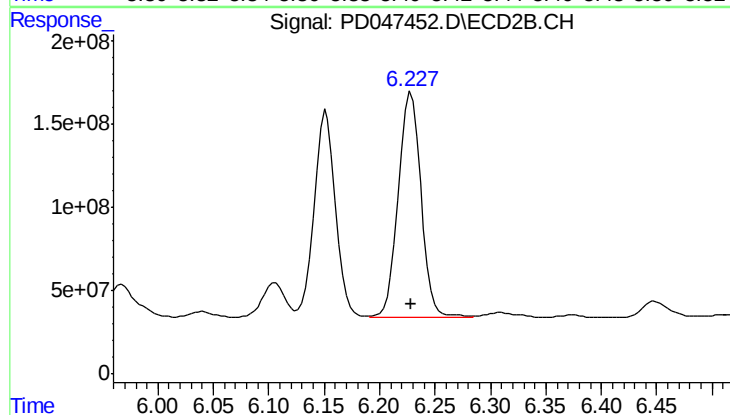


#26 Chlordane-4

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 1904448734
Conc: 489.85 ng/ml

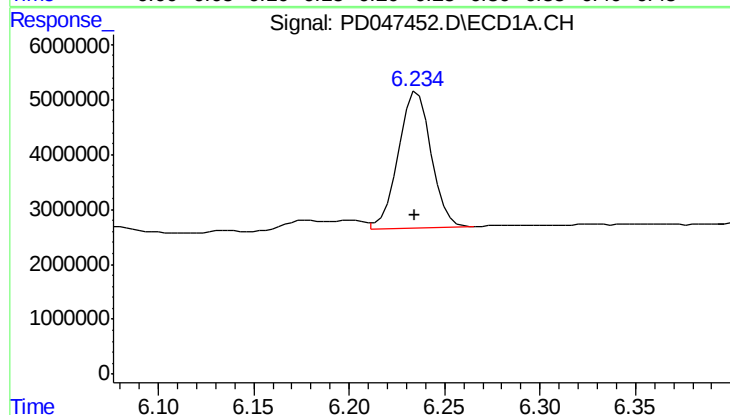


#27 Chlordane-5

R.T.: 6.236 min
Delta R.T.: 0.001 min
Response: 30150579
Conc: 514.00 ng/ml

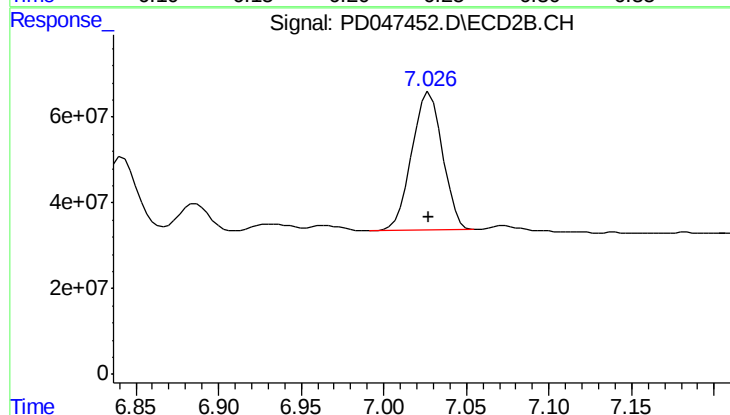

#27 Chlordane-5


R.T.: 7.028 min
Delta R.T.: 0.000 min
Response: 418412149
Conc: 500.21 ng/ml

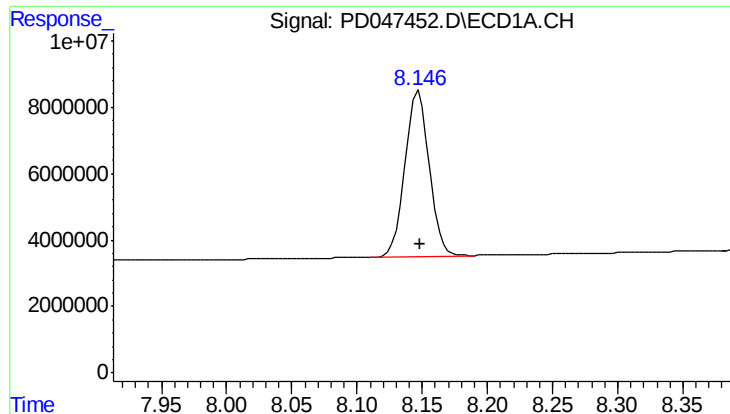

#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 64317731
Conc: 49.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD050518CHLOR

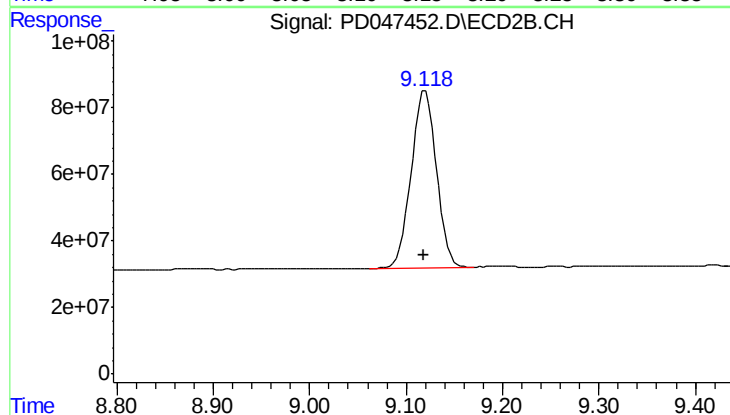

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 958125518
Conc: 48.03 ng/ml