

Data Path : P:\HPCHEM1\ECD D\Data\PD050518\
 Data File : PD047445.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2018 21:27
 Operator : UA/AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Manual Integrations
 APPROVED

UGO
 5/7/2018 10:32:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:45:11 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD050518.M
 Quant Title : GC Extractables
 QLast Update : Fri May 04 23:32:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.041	127.2E6	1721.4E6	101.095	97.693
28)	SA Decachlor...	8.147	9.120	126.0E6	1778.6E6	99.539	96.219
Target Compounds							
23)	Chlordane-1	4.288	5.040	54986856	960.1E6	998.140	974.357m
24)	Chlordane-2	4.784	5.507	55065772	899.3E6	993.364	960.464
25)	Chlordane-3	5.345	6.152	161.1E6	3138.1E6	957.972m	978.130
26)	Chlordane-4	5.404	6.229	154.3E6	3576.5E6	1008.598	976.929
27)	Chlordane-5	6.236	7.028	59166540	786.5E6	997.519	978.584

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD D\Data\PD050518\
Data File : PD047445.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2018 21:27
Operator : UA/AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleID :
PCHLORICC1000


Manual Integrations
APPROVED

UGO
5/7/2018 10:32:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:45:11 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD050518.M
Quant Title : GC Extractables
QLast Update : Fri May 04 23:32:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

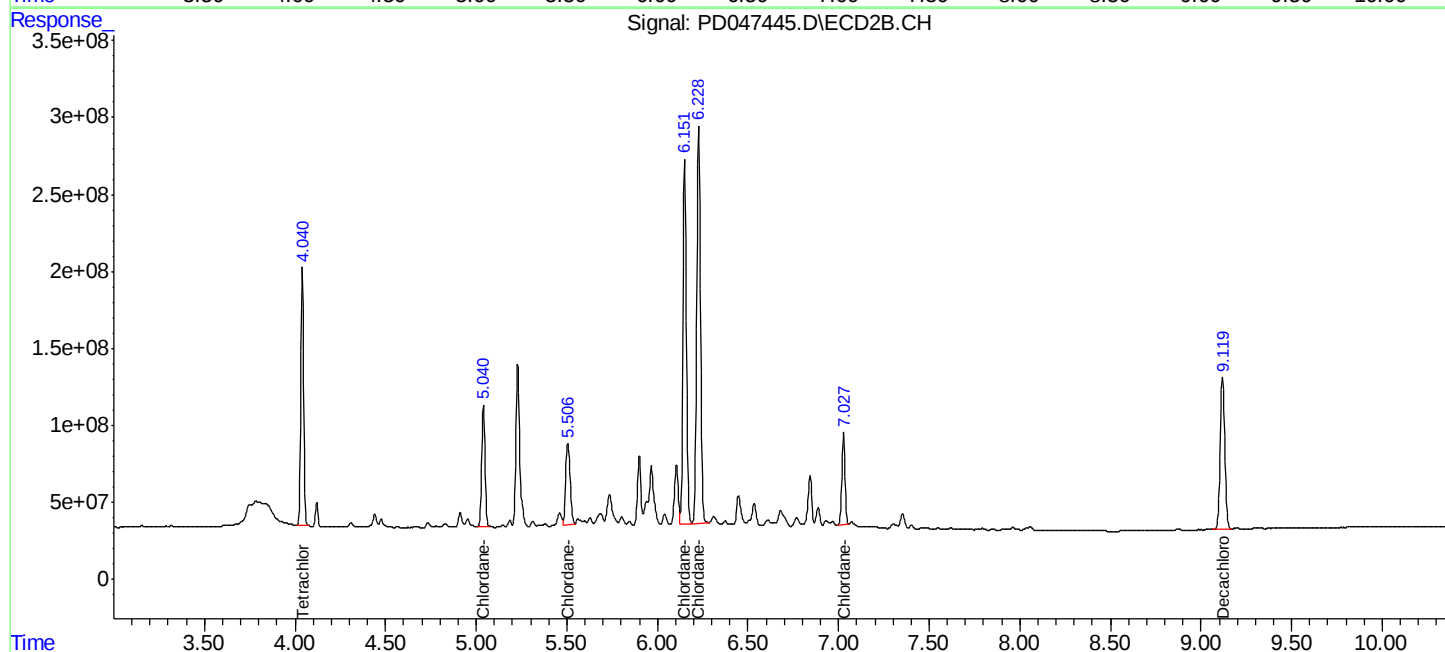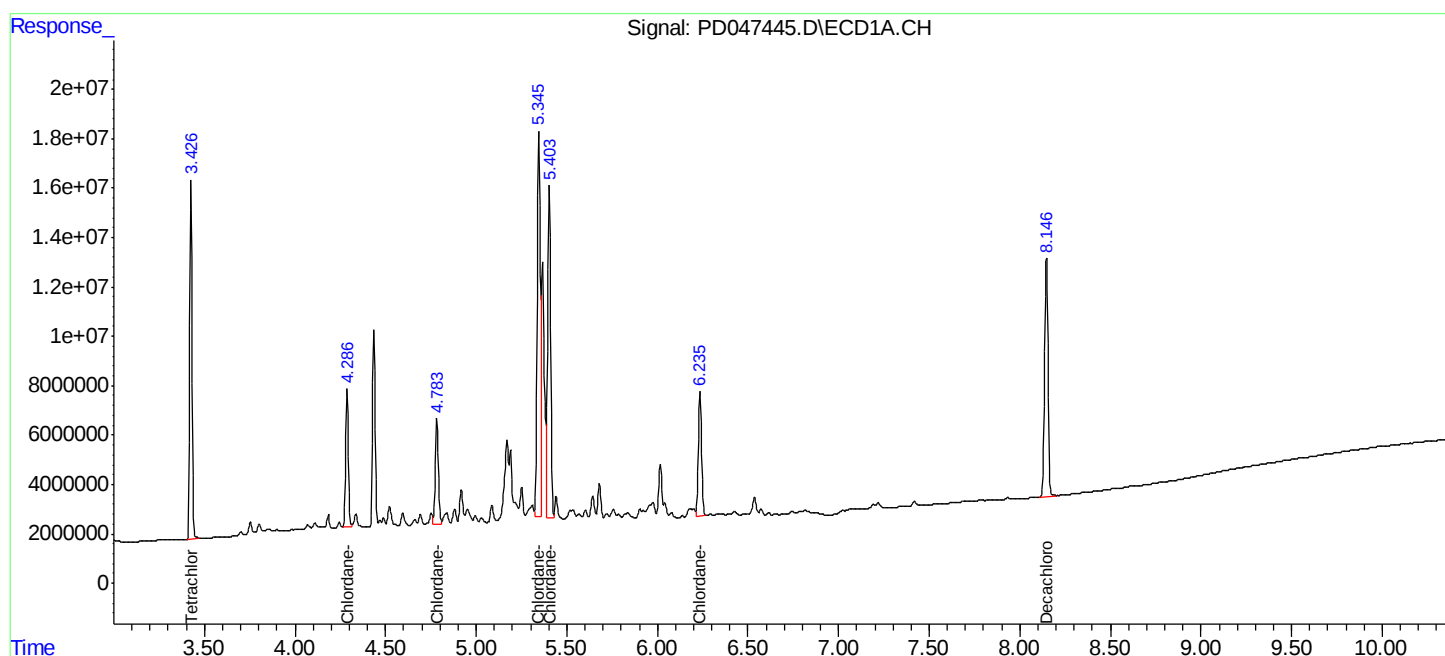

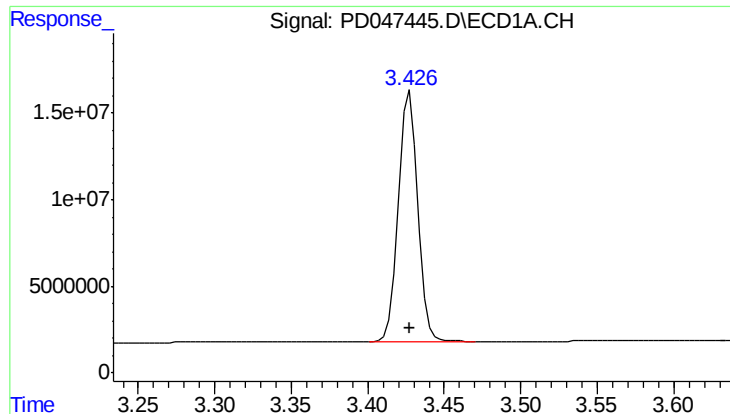


#1 Tetrachloro-m-xylene

R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 127172766
Conc: 101.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000


Manual Integrations
APPROVED

UGO
5/7/2018 10:32:51 AM

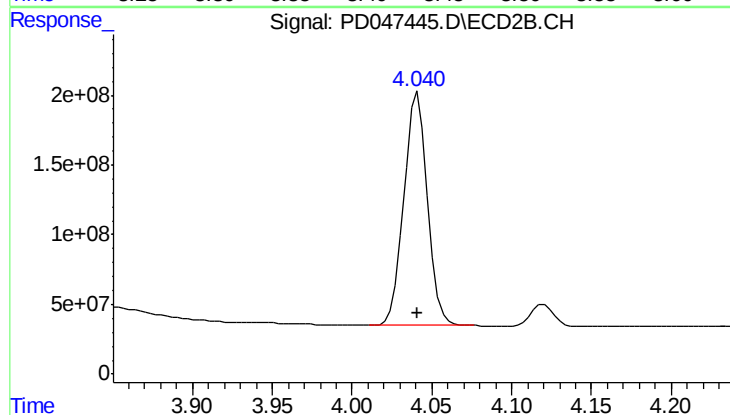


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: 0.000 min
Response: 1721372012
Conc: 97.69 ng/ml

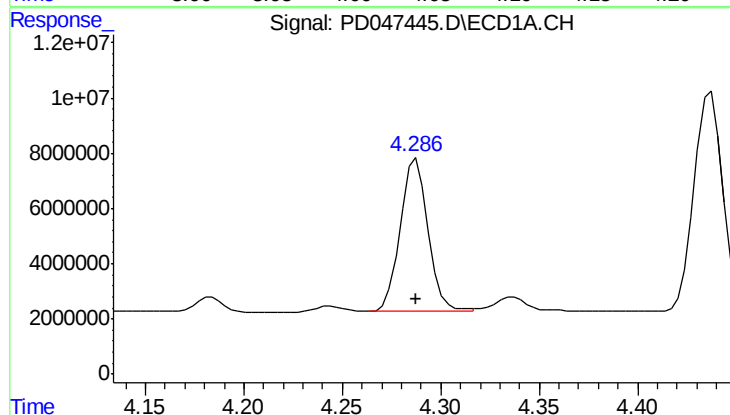


#23 Chlordane-1

R.T.: 4.288 min
Delta R.T.: 0.000 min
Response: 54986856
Conc: 998.14 ng/ml

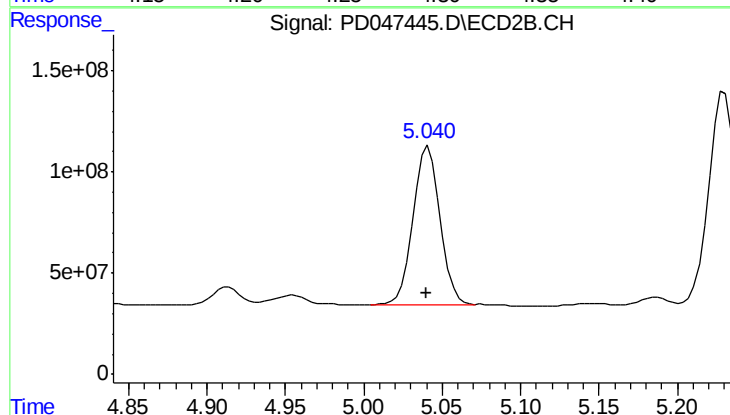

#23 Chlordane-1

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 960093368
Conc: 974.36 ng/ml m

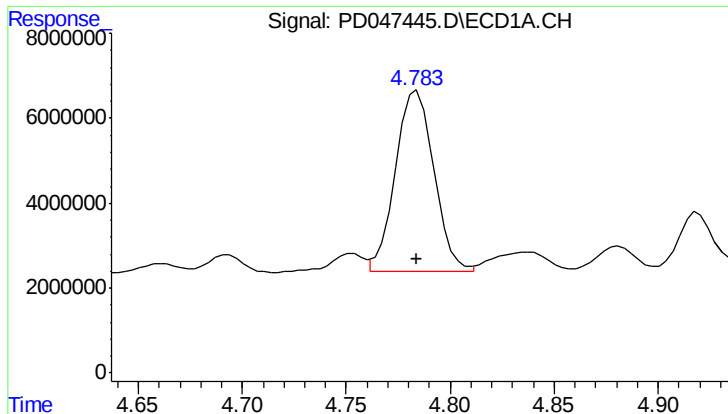


#24 Chlordane-2

R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 55065772
Conc: 993.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000


Manual Integrations
APPROVED

UGO
5/7/2018 10:32:51 AM

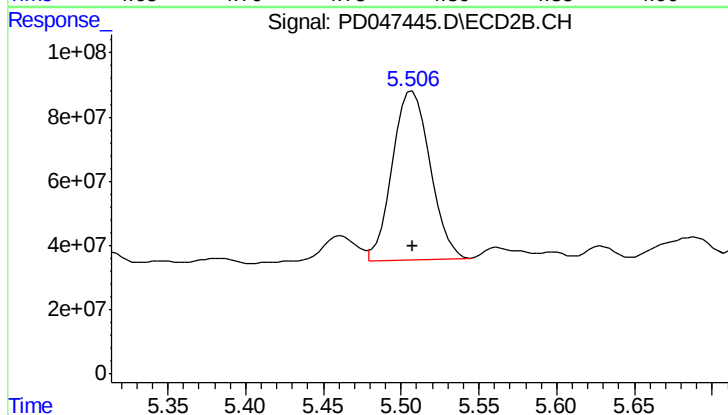


#24 Chlordane-2

R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 899316919
Conc: 960.46 ng/ml

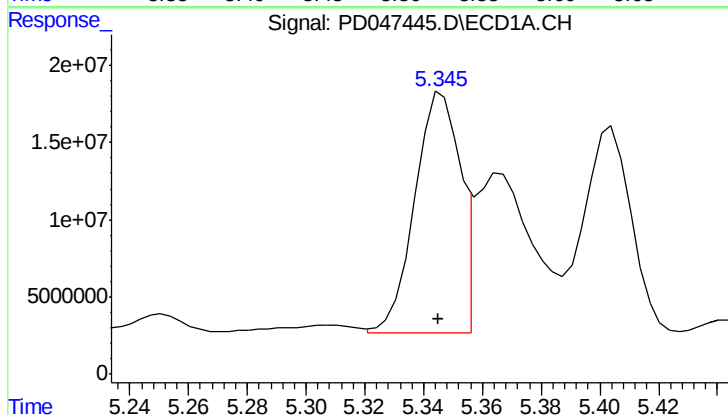


#25 Chlordane-3

R.T.: 5.345 min
Delta R.T.: 0.000 min
Response: 161061607
Conc: 957.97 ng/ml m

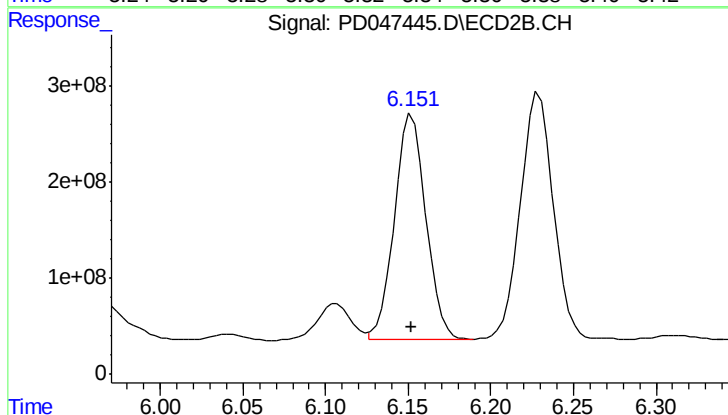

#25 Chlordane-3

R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 3138118914
Conc: 978.13 ng/ml

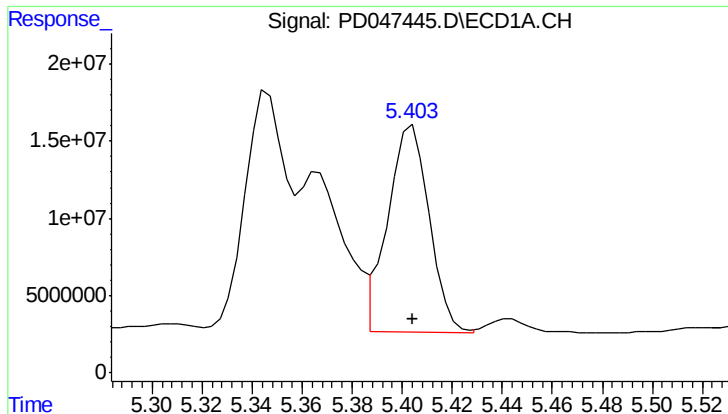


#26 Chlordane-4

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 154269359
Conc: 1008.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000


Manual Integrations
APPROVED

UGO
5/7/2018 10:32:51 AM

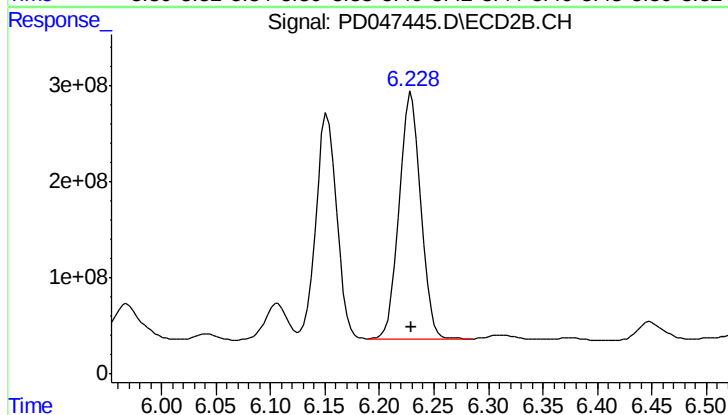


#26 Chlordane-4

R.T.: 6.229 min
Delta R.T.: 0.000 min
Response: 3576499672
Conc: 976.93 ng/ml

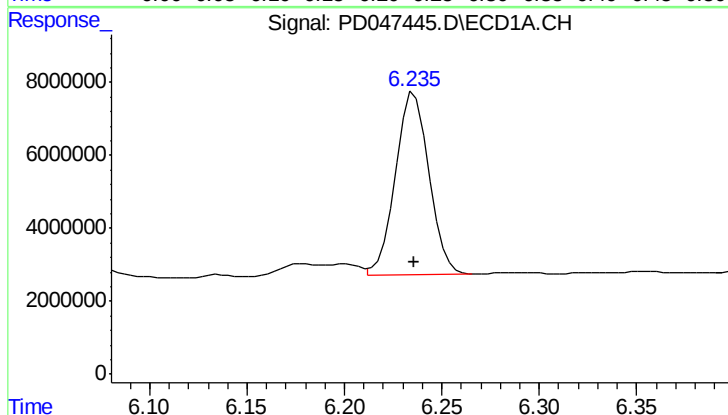


#27 Chlordane-5

R.T.: 6.236 min
Delta R.T.: 0.000 min
Response: 59166540
Conc: 997.52 ng/ml

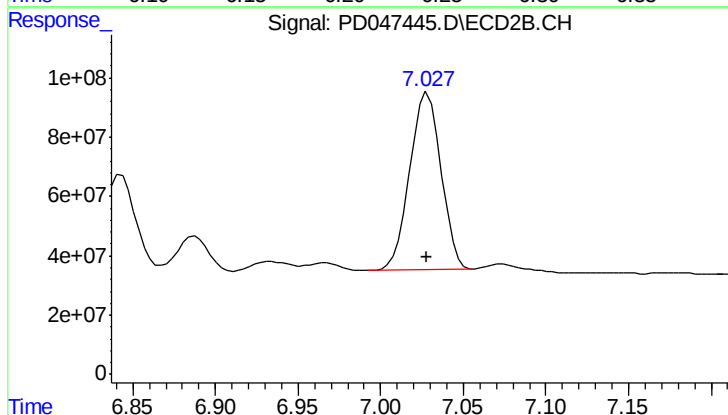

#27 Chlordane-5

R.T.: 7.028 min
Delta R.T.: 0.000 min
Response: 786524850
Conc: 978.58 ng/ml

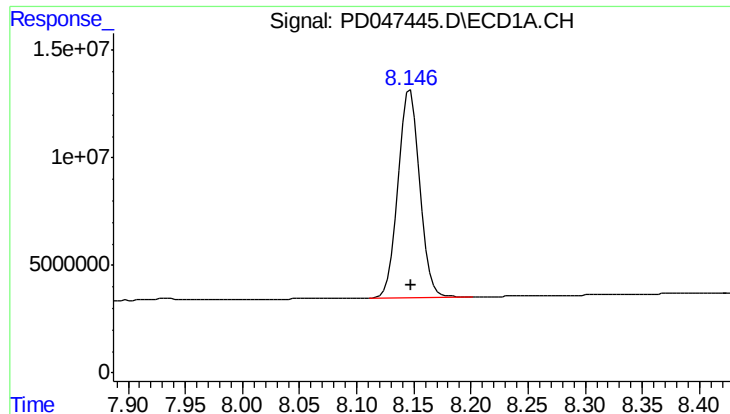


#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 126032821
Conc: 99.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Manual Integrations
APPROVED

UGO
5/7/2018 10:32:51 AM

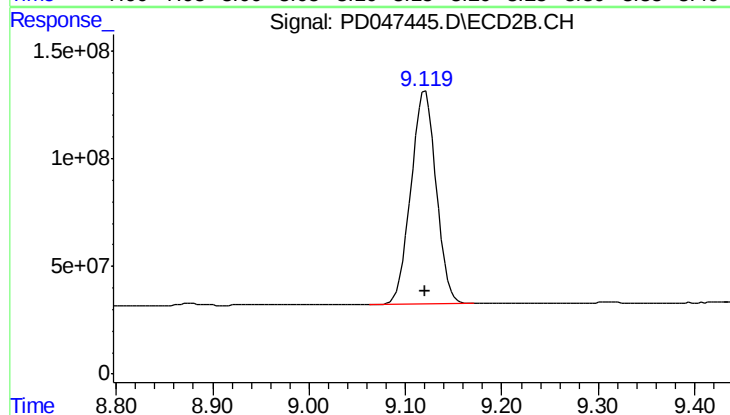

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 1778645411
Conc: 96.22 ng/ml