

Data Path : P:\HPCHEM1\ECD D\Data\PD050518\
 Data File : PD047446.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 May 2018 21:42
 Operator : UA/AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Manual Integrations
 APPROVED

UGO
 5/7/2018 10:32:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:48:18 2018
 Quant Method : P:\HPCHEM1\ECD_D\Method\PD050518.M
 Quant Title : GC Extractables
 QLast Update : Fri May 04 23:35:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.041	94870905	1319.4E6	75.278	74.920
28)	SA Decachlor...	8.147	9.119	95241473	1381.8E6	75.147	74.833
Target Compounds							
23)	Chlordane-1	4.288	5.039	41472240	741.2E6	751.876	751.746m
24)	Chlordane-2	4.784	5.507	41770219	701.0E6	752.341	749.138
25)	Chlordane-3	5.344	6.152	132.3E6	2412.0E6	770.069m	751.193
26)	Chlordane-4	5.404	6.229	115.0E6	2752.0E6	751.209	751.146
27)	Chlordane-5	6.235	7.027	44793517	607.7E6	753.456	754.065

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD D\Data\PD050518\
Data File : PD047446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 May 2018 21:42
Operator : UA/AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleID :
PCHLORICC750


Manual Integrations
APPROVED

UGO
5/7/2018 10:32:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:48:18 2018
Quant Method : P:\HPCHEM1\ECD_D\Method\PD050518.M
Quant Title : GC Extractables
QLast Update : Fri May 04 23:35:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

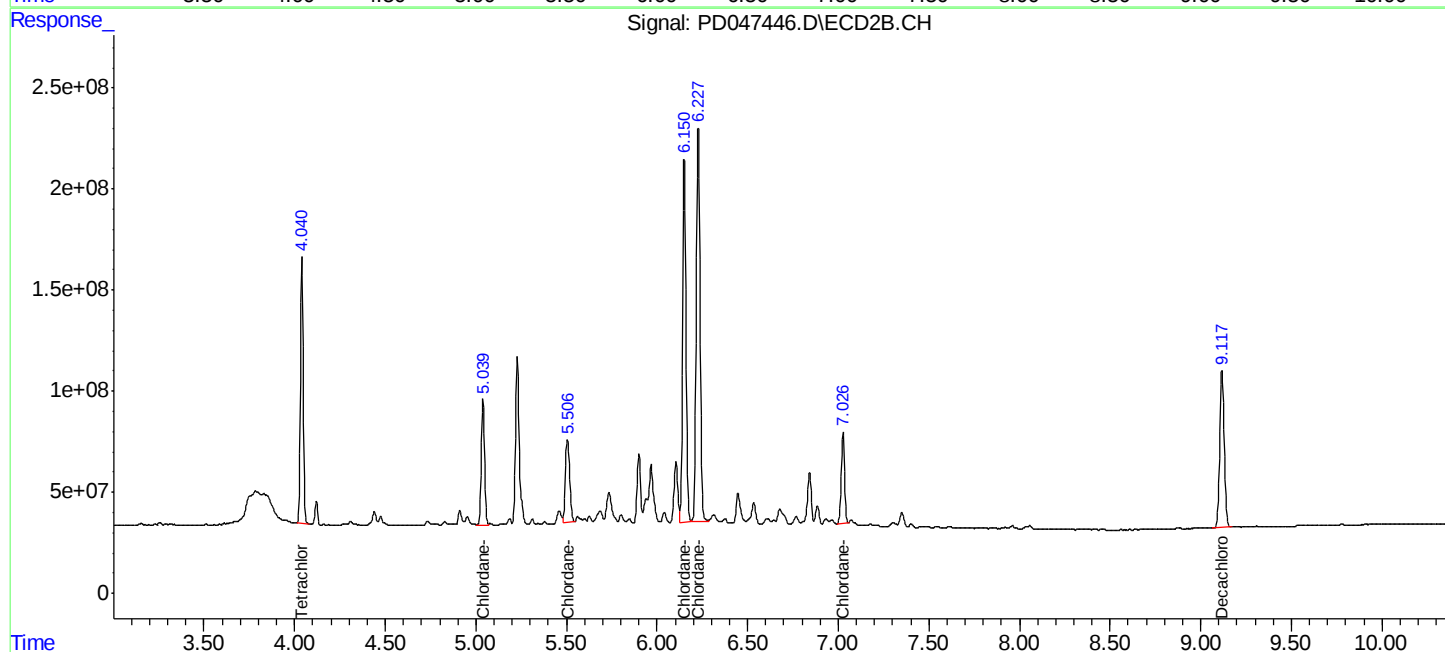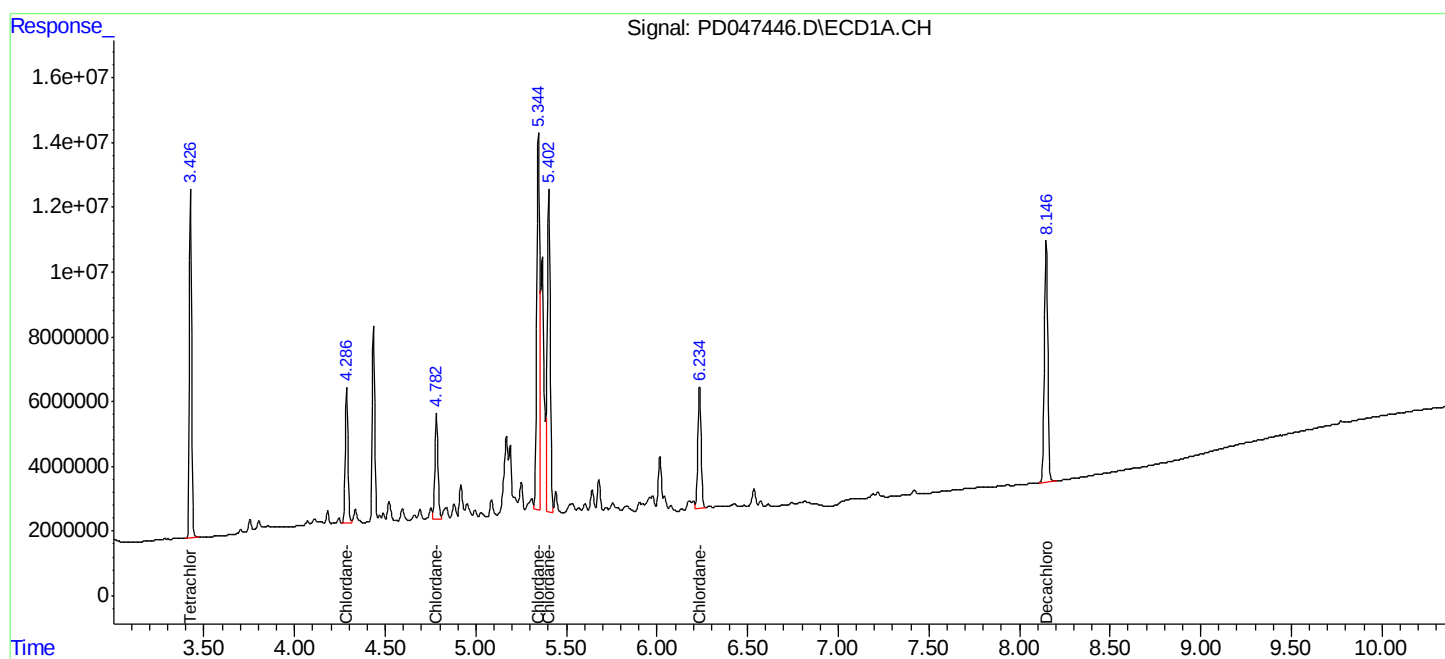

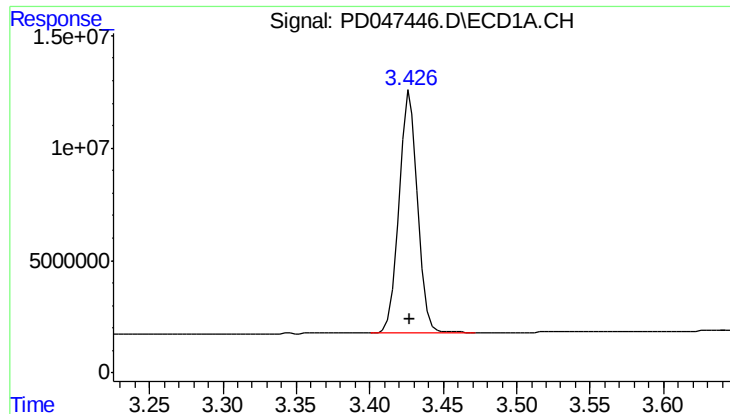


#1 Tetrachloro-m-xylene

R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 94870905
Conc: 75.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

UGO
5/7/2018 10:32:48 AM

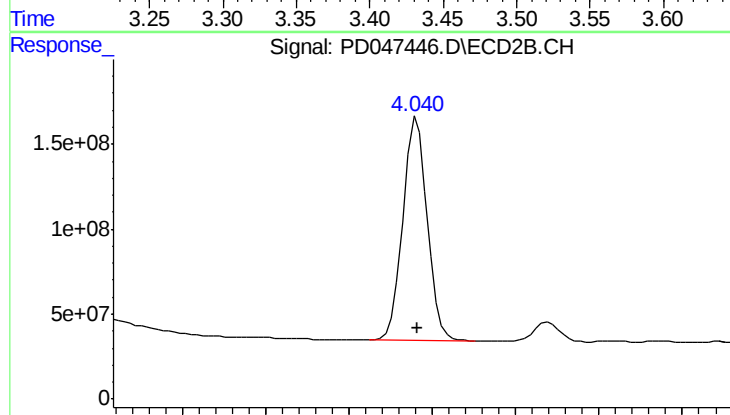


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: 0.000 min
Response: 1319394688
Conc: 74.92 ng/ml

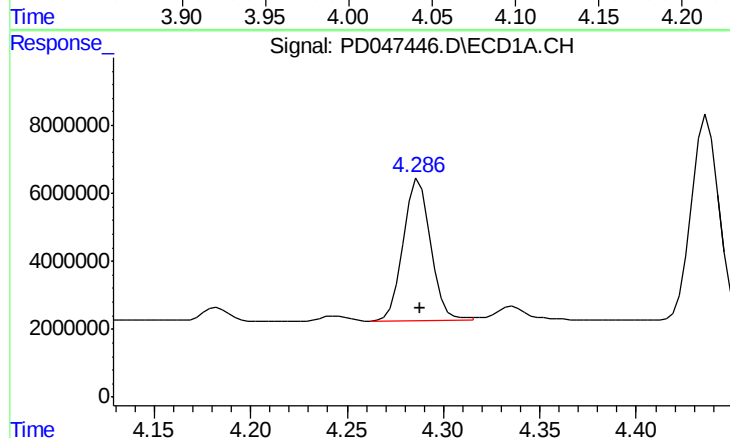


#23 Chlordane-1

R.T.: 4.288 min
Delta R.T.: 0.000 min
Response: 41472240
Conc: 751.88 ng/ml

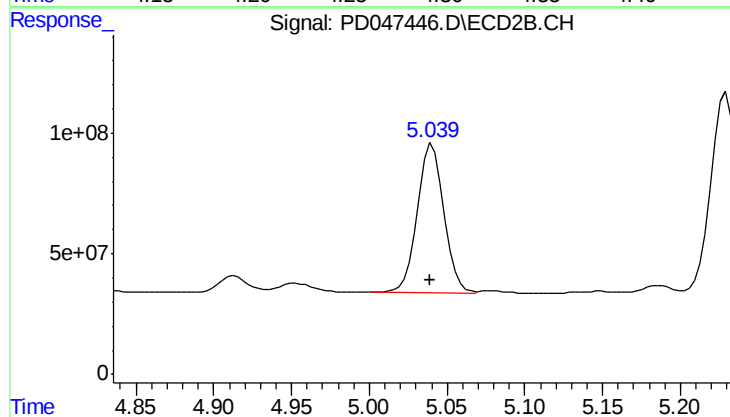

#23 Chlordane-1

R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 741234228
Conc: 751.75 ng/ml m

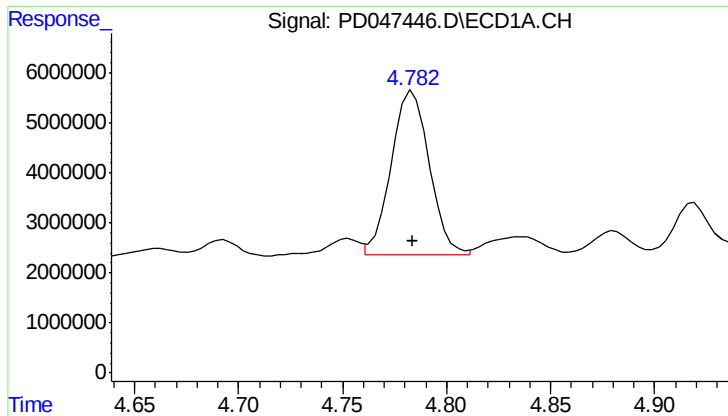


#24 Chlordane-2

R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 41770219
Conc: 752.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

UGO
5/7/2018 10:32:48 AM

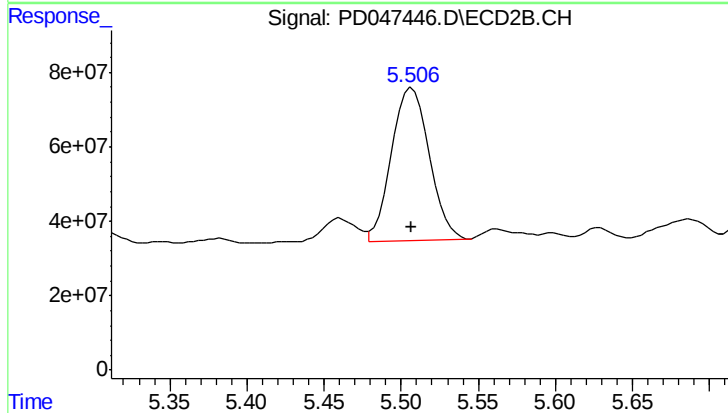


#24 Chlordane-2

R.T.: 5.507 min
Delta R.T.: 0.000 min
Response: 701041158
Conc: 749.14 ng/ml

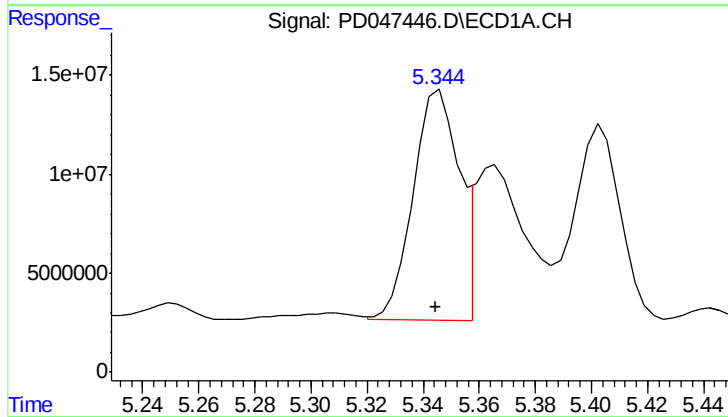


#25 Chlordane-3

R.T.: 5.344 min
Delta R.T.: 0.000 min
Response: 132262696
Conc: 770.07 ng/ml m

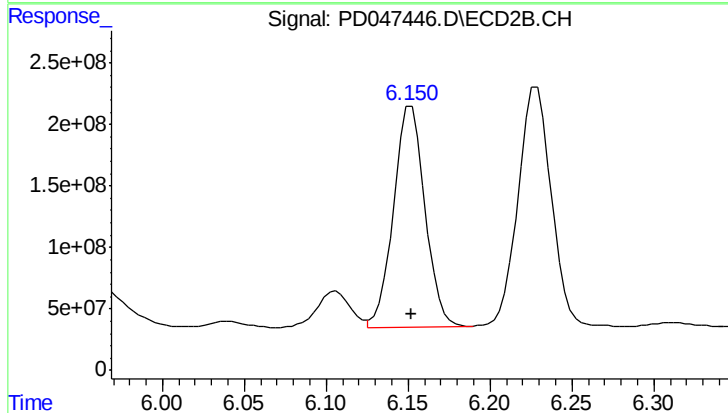

#25 Chlordane-3

R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 2411960827
Conc: 751.19 ng/ml

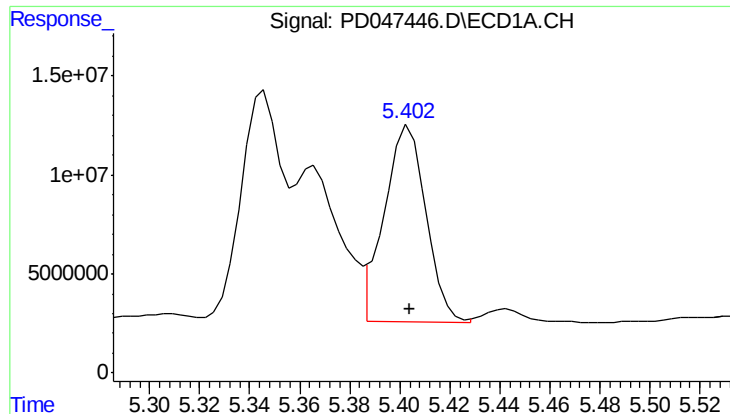


#26 Chlordane-4

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 114993269
Conc: 751.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

UGO
5/7/2018 10:32:48 AM

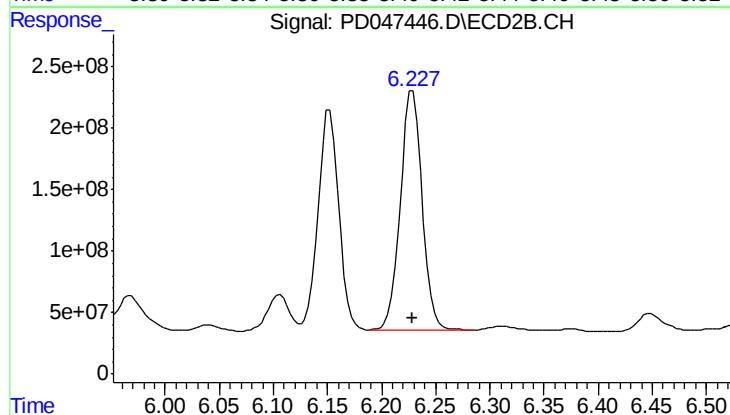


#26 Chlordane-4

R.T.: 6.229 min
Delta R.T.: 0.000 min
Response: 2752019369
Conc: 751.15 ng/ml

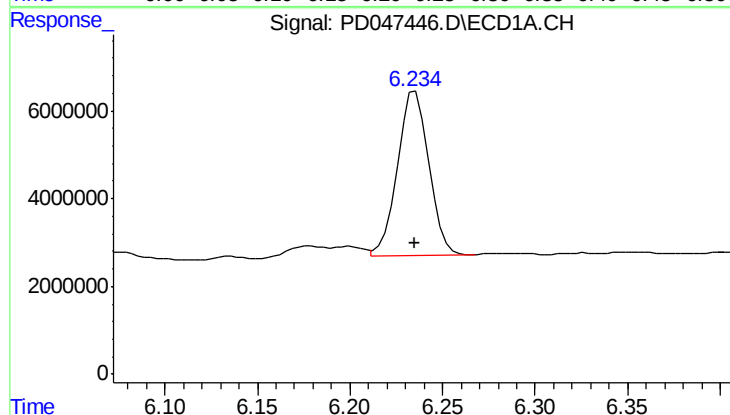


#27 Chlordane-5

R.T.: 6.235 min
Delta R.T.: 0.000 min
Response: 44793517
Conc: 753.46 ng/ml

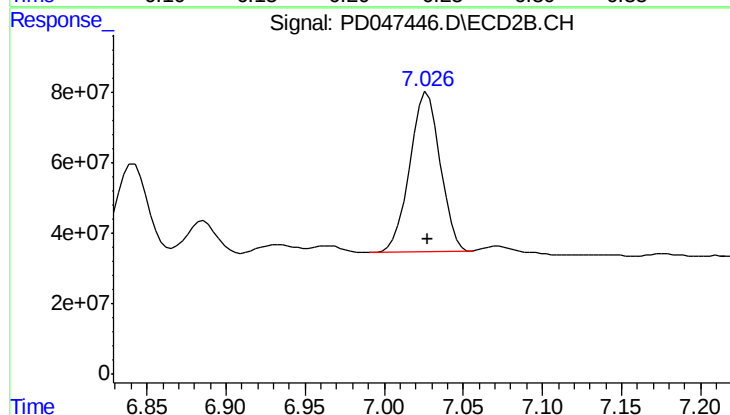

#27 Chlordane-5

R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 607717543
Conc: 754.06 ng/ml

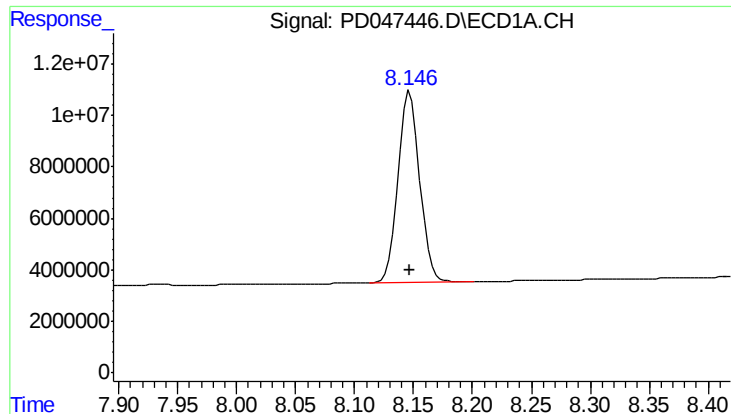


#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 95241473
Conc: 75.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Manual Integrations
APPROVED

UGO
5/7/2018 10:32:48 AM

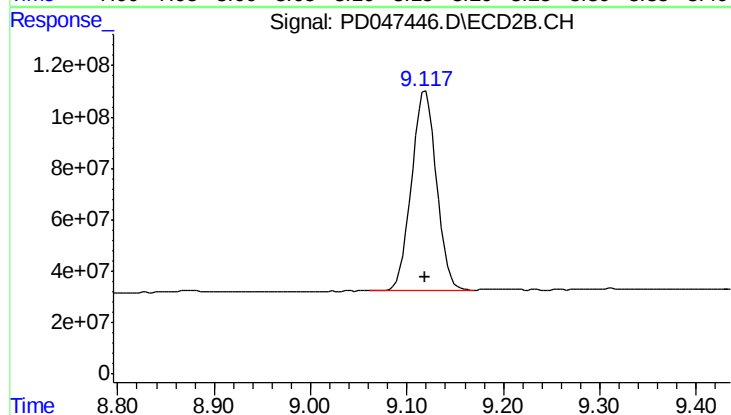

#28 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 1381765084
Conc: 74.83 ng/ml