

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050521\
 Data File : PD062712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 10:03
 Operator : AR\AJ
 Sample : M2232-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5A9

Manual Integrations
 APPROVED

Ankita
 5/6/2021 4:15:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 01:42:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 30 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	3.958	8523038	2241.6E6	8.902m	184.597m#
27)	SA Decachlor...	8.208	9.033	14556898	154.8E6	13.562	14.182m
Target Compounds							
10)	B trans-Chl...	5.391	6.083	935048	37839136	0.746m	2.310m#
11)	B cis-Chlor...	5.446	6.154	946599	18766830	0.771	1.209 #
15)	B Endosulfa...	6.285	6.899	768907	11709069	0.741m	0.936m#
16)	A 4,4'-DDD	6.126	6.798	1084399	19890363	1.089m	1.600m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050521\
Data File : PD062712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 10:03
Operator : AR\AJ
Sample : M2232-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:42:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Apr 30 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

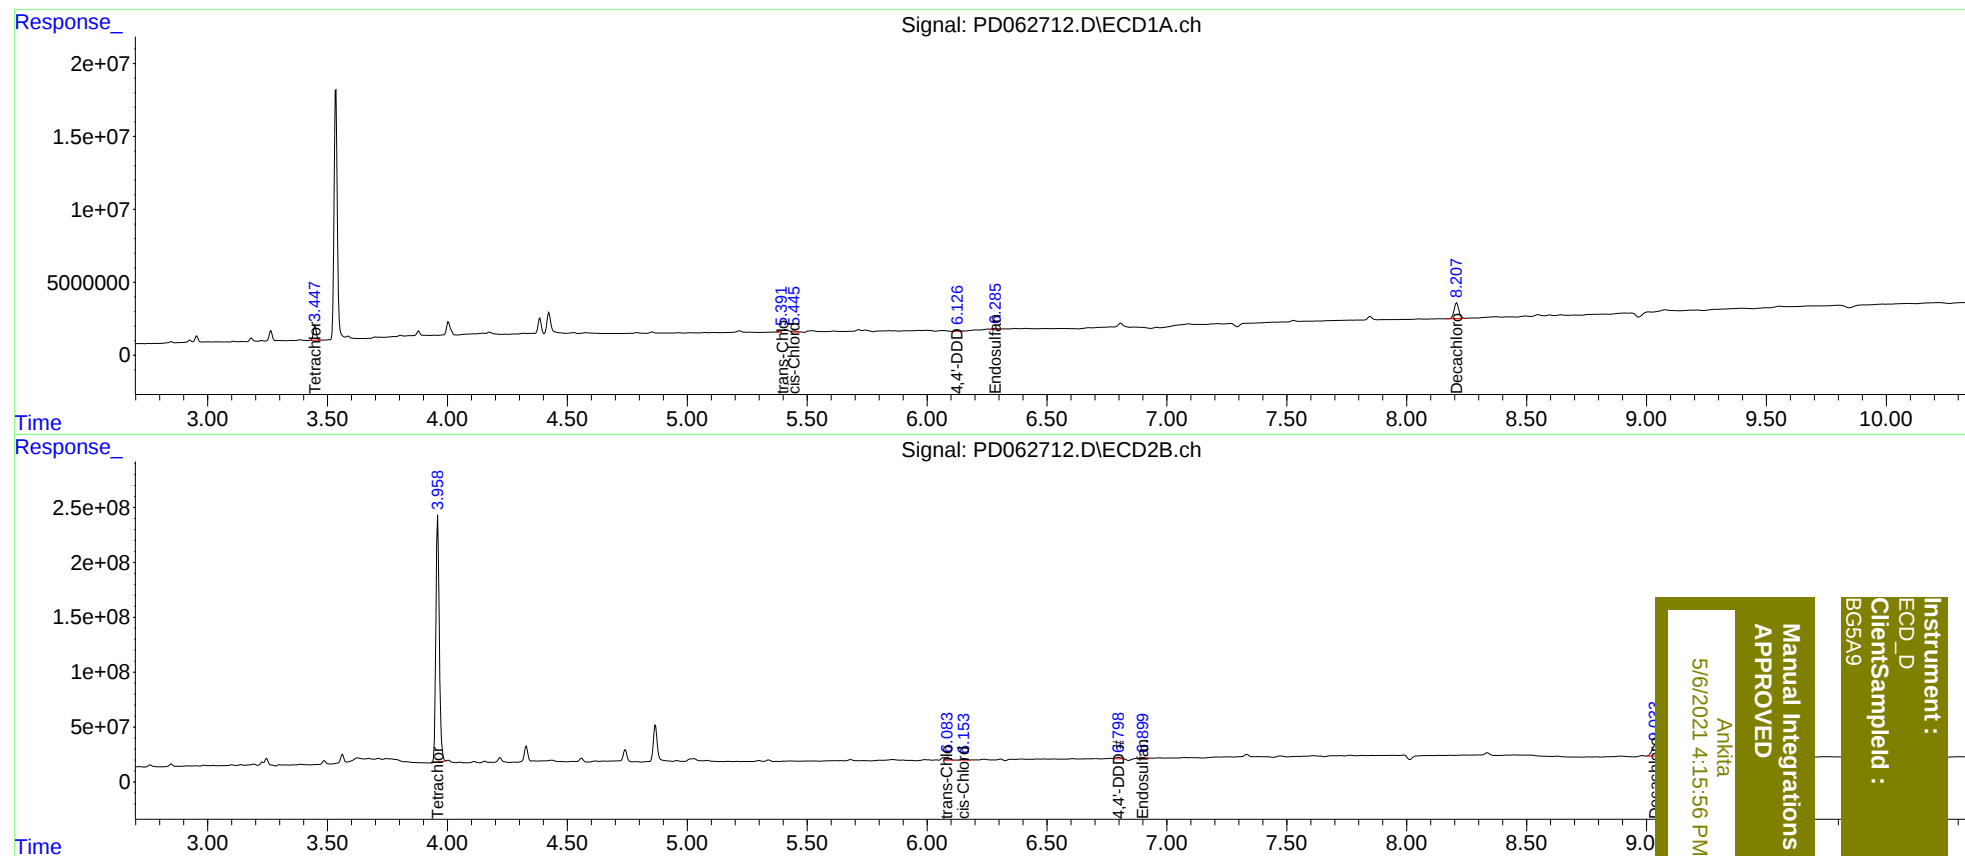

Manual Integrations
APPROVED

Ankita

5/6/2021 4:15:56 PM

Instrument :
ECD_D
ClientSampleId :
BG5A9