

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
 Data File : PD075262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 13:33
 Operator : AR\AJ
 Sample : 02479-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW953

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/09/2023
 Supervised By : Ankita Jodhani 05/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 00:23:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.772	45591446	9690767	19.989	9.188 #
27) SA Decachlor...	9.078	7.915	114.7E6	30621472	46.336	32.425 #
Target Compounds						
3) MA gamma-BHC...	4.343	3.614	391.6E6	26389585	108.920m	17.953 #
15) B Endosulfa...	6.839	5.919	23193.6E6	1097.2E6	7202.112m	857.504m#
17) MA 4,4'-DDT	7.015	6.033	3987.0E6	1525.7E6	1570.766m	1513.816
19) B Endosulfa...	7.156	6.331	250.2E6	143.9E6	90.953m	123.690m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
Data File : PD075262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 13:33
Operator : AR\AJ
Sample : 02479-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 00:23:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

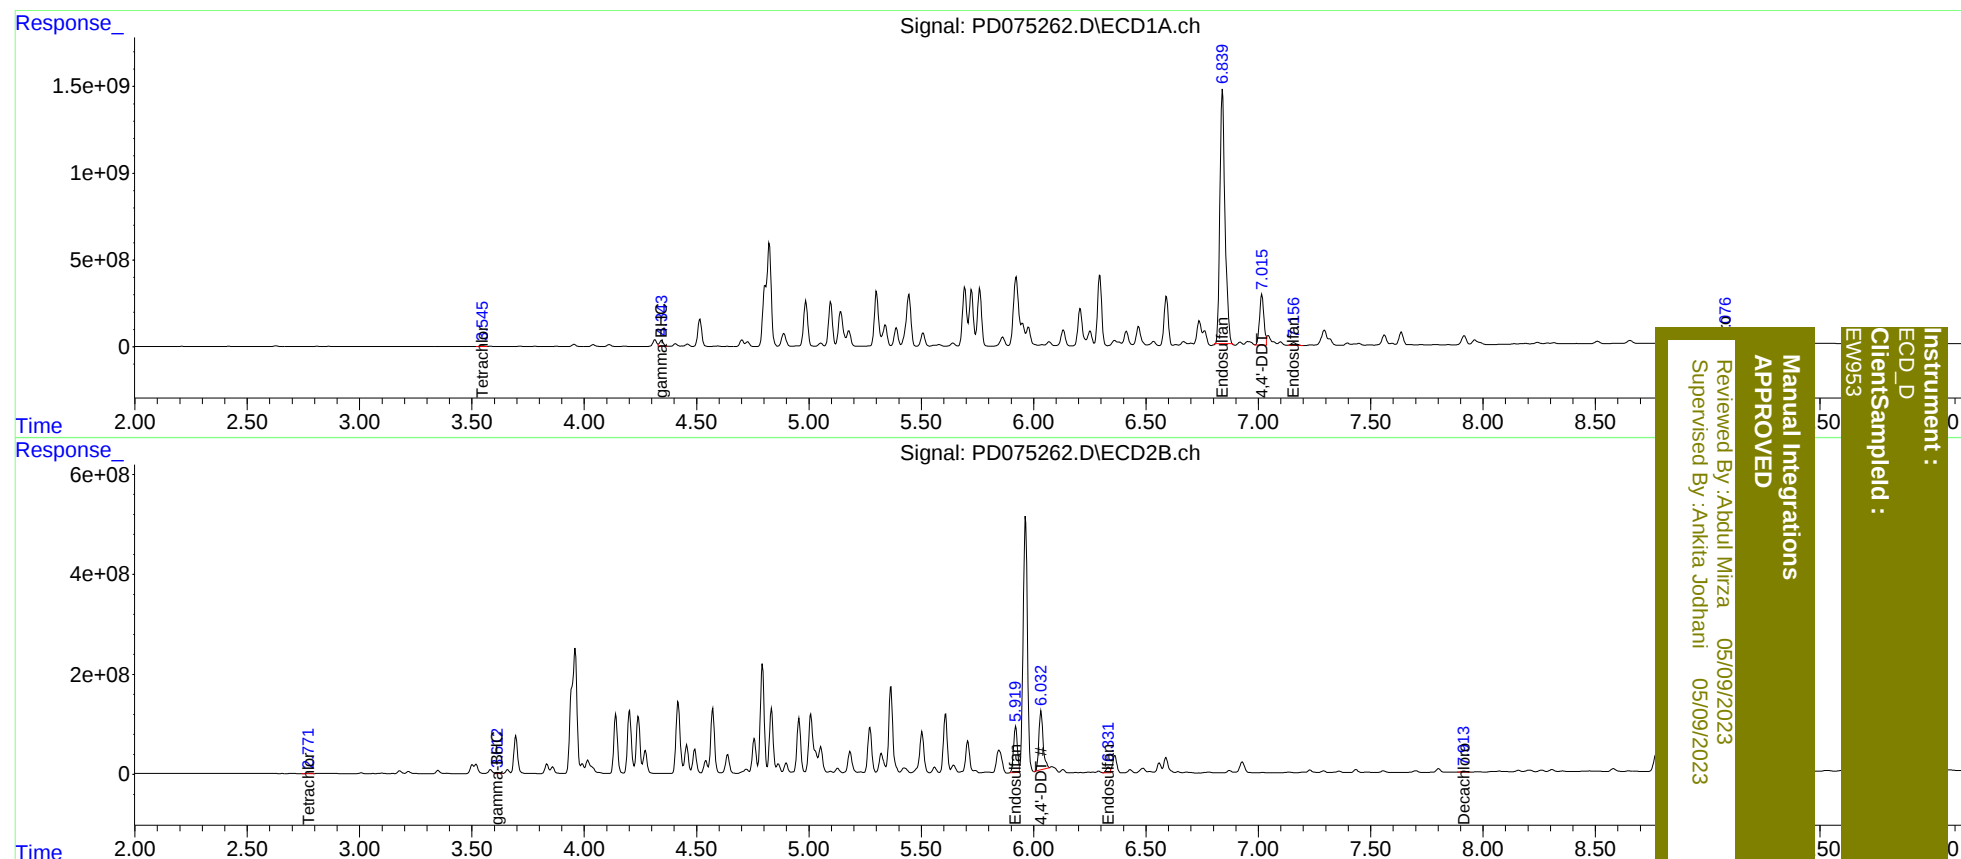

Reviewed By: Abdul Mirza 05/09/2023
Supervised By: Ankita Jodhani 05/09/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW/953