

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
 Data File : PD075272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 17:17
 Operator : AR\AJ
 Sample : PB152520BS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS520

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/06/2023
 Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 00:26:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.771	43574686	20090220	19.105	19.048
2)	SA Decachlor...	9.088	7.917	84523145	29356645	34.155	31.085
Target Compounds							
2)	A alpha-BHC	4.004	3.273	15357729	6099625	3.994	3.938
3)	MA gamma-BHC...	4.338	3.603	14156746	5877797	3.938	3.999
4)	MA Heptachlor	4.929	3.944	14566591	6022418	3.907	4.122
5)	MB Aldrin	5.272	4.224	15201022	6219550	4.167	4.194
6)	B beta-BHC	4.534	3.900	6660897	2934721	4.058	4.030
7)	B delta-BHC	4.782	4.131	14408201	5465458	4.263	3.459
8)	B Heptachlo...	5.699	4.726	16305970	5636445	4.811	4.041
9)	A Endosulfan I	6.086	5.097	12128723	5144084	4.021	4.286
10)	B trans-Chl...	5.956	4.977	12391737	5744266	3.782	4.210
11)	B cis-Chlor...	6.035	5.041	12883453	5915632	3.780	4.239
12)	B 4,4'-DDE	6.207	5.231	25665811	9946287	7.859	7.737
13)	MA Dieldrin	6.362	5.362	28484270	10901430	8.329	7.990
14)	MA Endrin	6.593	5.636	20089852	8961671	6.947	7.368m
15)	B Endosulfa...	6.812	5.931	27248093	9175245	8.461	7.171
16)	A 4,4'-DDD	6.725	5.785	24075197	8570064	9.963	8.645
17)	MA 4,4'-DDT	7.041	6.037	18086498	6536206	7.126	6.485
18)	B Endrin al...	6.941	6.111	18774214	6821345	7.936	6.717
19)	B Endosulfa...	7.177	6.334	20933832	8513170	7.610	7.320
20)	A Methoxychlor	7.516	6.612	53551261	21800334	36.456	38.060
21)	B Endrin ke...	7.663	6.840	23479836	9777406	7.746	7.415

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
Data File : PD075272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 17:17
Operator : AR\AJ
Sample : PB152520BS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 00:26:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

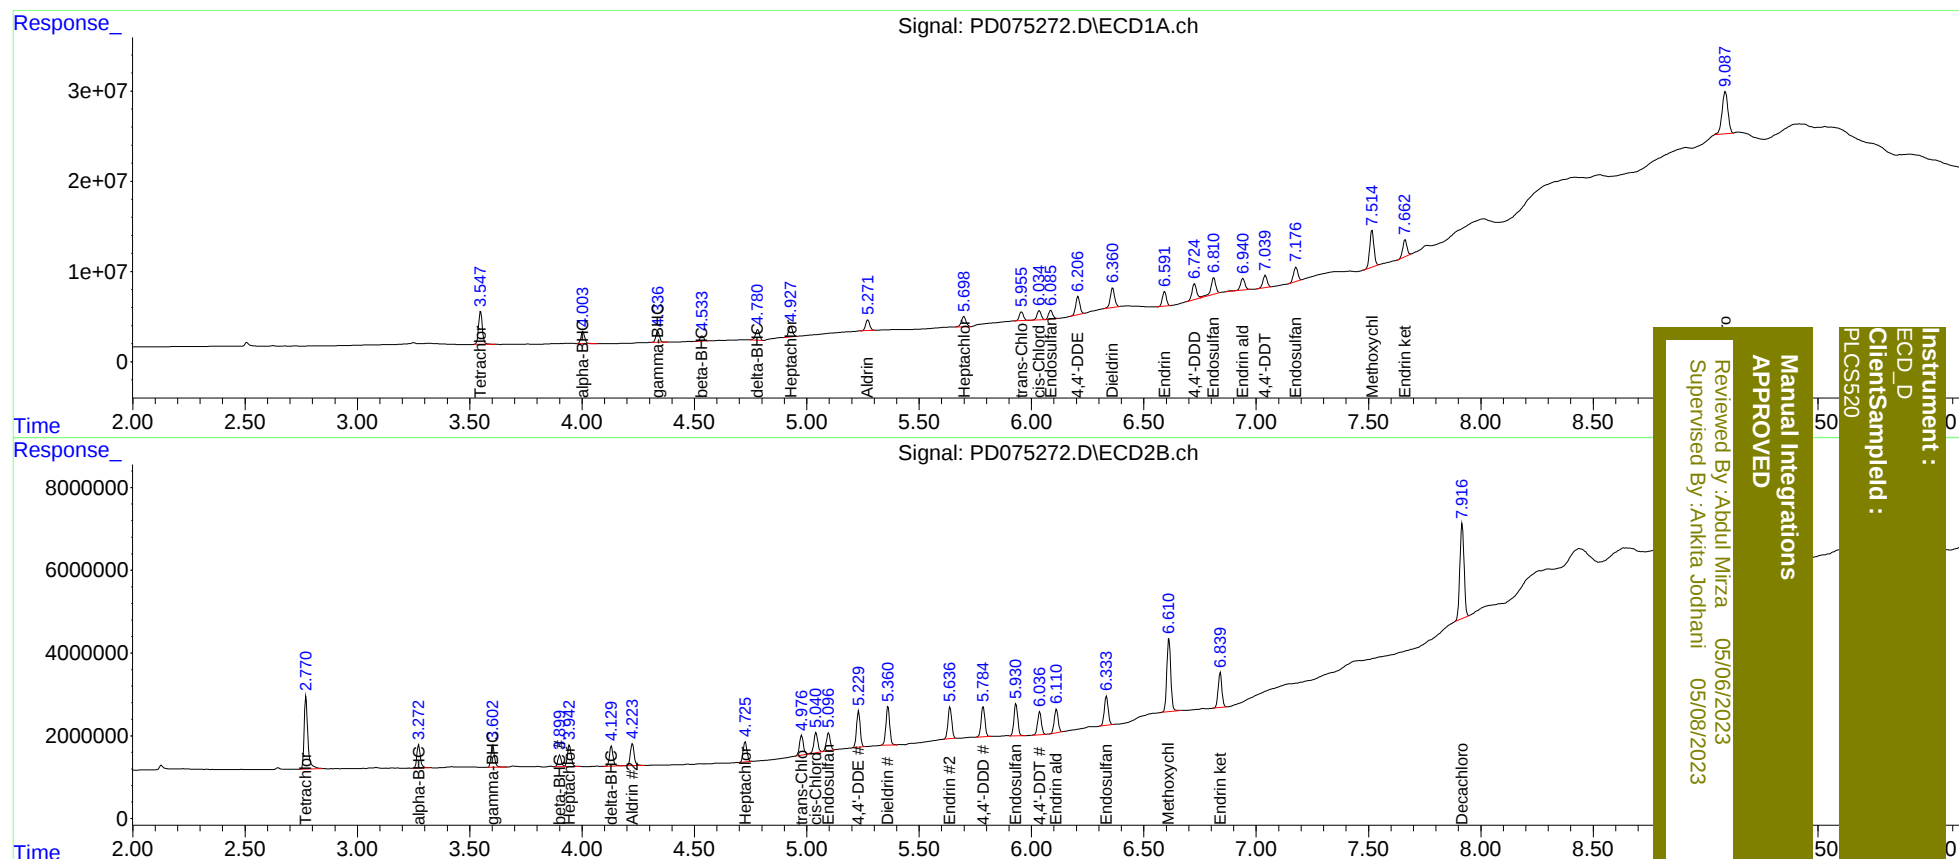

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Instrument :
ECD_D
Client Sampled :
PLCS520