

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
 Data File : PD075280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 20:26
 Operator : AR\AJ
 Sample : 02479-03DL 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW944DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/06/2023
 Supervised By : Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 00:27:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.771	8482095	2297191	3.719m	2.178 #
2) SA Decachlor...	9.085	7.916	8637272	4060167	3.490	4.299
Target Compounds						
7) B delta-BHC	4.801	4.140	171.7E6	78165896	50.805m	49.469
17) MA 4,4'-DDT	7.012	6.031	157.5E6	75548692	62.057m	74.959
19) B Endosulfa...	7.155	6.330	7632631	6048372	2.775m	5.201m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
Data File : PD075280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 20:26
Operator : AR\AJ
Sample : 02479-03DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 00:27:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

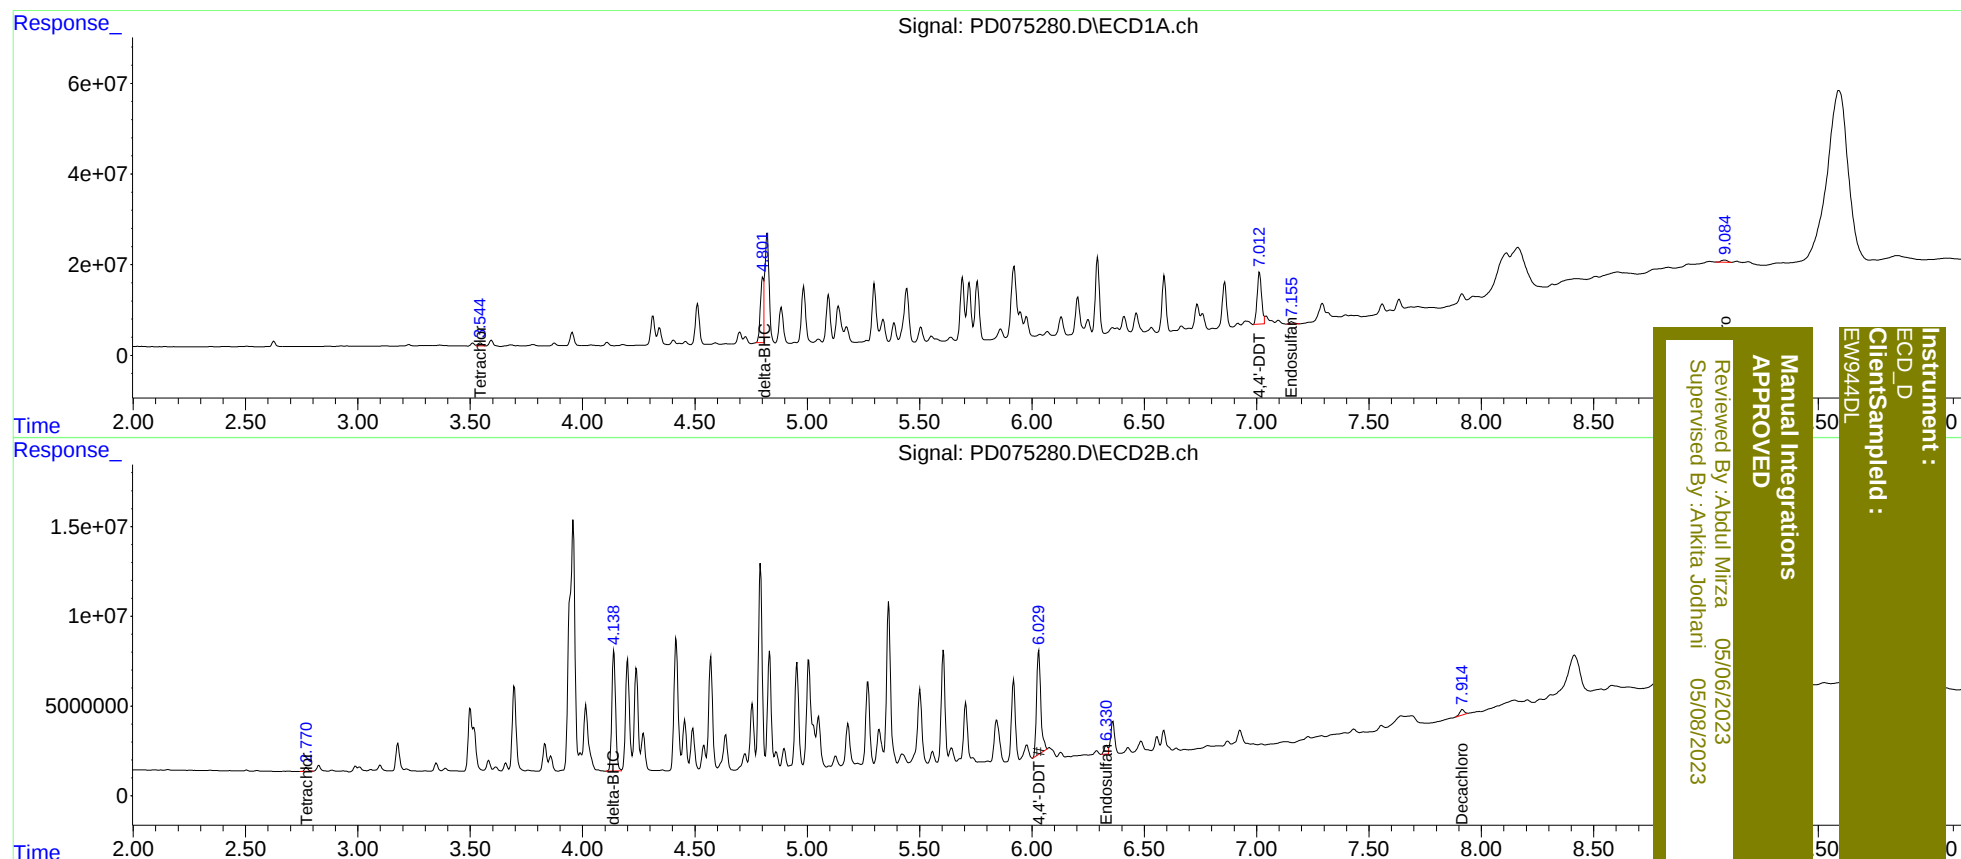

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Instrument :
ECD_D
Client Sampled :
EW944DL