

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
 Data File : PD075287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 22:28
 Operator : AR\AJ
 Sample : PB152594BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS594

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 00:28:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.549	2.771	44195331	20263234	19.377	19.212
27) SA Decachlor...	9.086	7.916	85532975	31199395	34.563	33.037
Target Compounds						
2) A alpha-BHC	4.004	3.273	15331167	6170250	3.987	3.983
3) MA gamma-BHC...	4.338	3.603	14548933	5798955	4.047	3.945
4) MA Heptachlor	4.929	3.944	15035078	6094632	4.033	4.171
5) MB Aldrin	5.272	4.224	15364167	6226343	4.212	4.198
6) B beta-BHC	4.534	3.900	7040923	2968419	4.289	4.077
7) B delta-BHC	4.782	4.130	13837229	5193630	4.094	3.287
8) B Heptachlo...	5.699	4.726	14608976	5653122	4.310	4.053
9) A Endosulfan I	6.086	5.097	12439807	5424476	4.124	4.520
10) B trans-Chl...	5.956	4.977	12945608	5863026	3.951	4.297
11) B cis-Chlor...	6.035	5.041	13328610	6052776	3.911	4.337
12) B 4,4'-DDE	6.207	5.230	24894740	10241377	7.623	7.966
13) MA Dieldrin	6.361	5.361	26579643	11467721	7.772	8.405
14) MA Endrin	6.592	5.637	22194545	8792597	7.675	7.229
15) B Endosulfa...	6.811	5.931	21817383	9725799	6.775	7.601
16) A 4,4'-DDD	6.725	5.785	21011697	9202630	8.695	9.283
17) MA 4,4'-DDT	7.040	6.036	17757370	6623597	6.996	6.572
18) B Endrin al...	6.941	6.111	17844436	7373407	7.543	7.261
19) B Endosulfa...	7.176	6.333	21476071	8758141	7.807	7.530
20) A Methoxychlor	7.515	6.612	52437754	21539818	35.698	37.605
21) B Endrin ke...	7.662	6.840	24048189	10421442	7.934	7.903

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
Data File : PD075287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 22:28
Operator : AR\AJ
Sample : PB152594BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 00:28:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

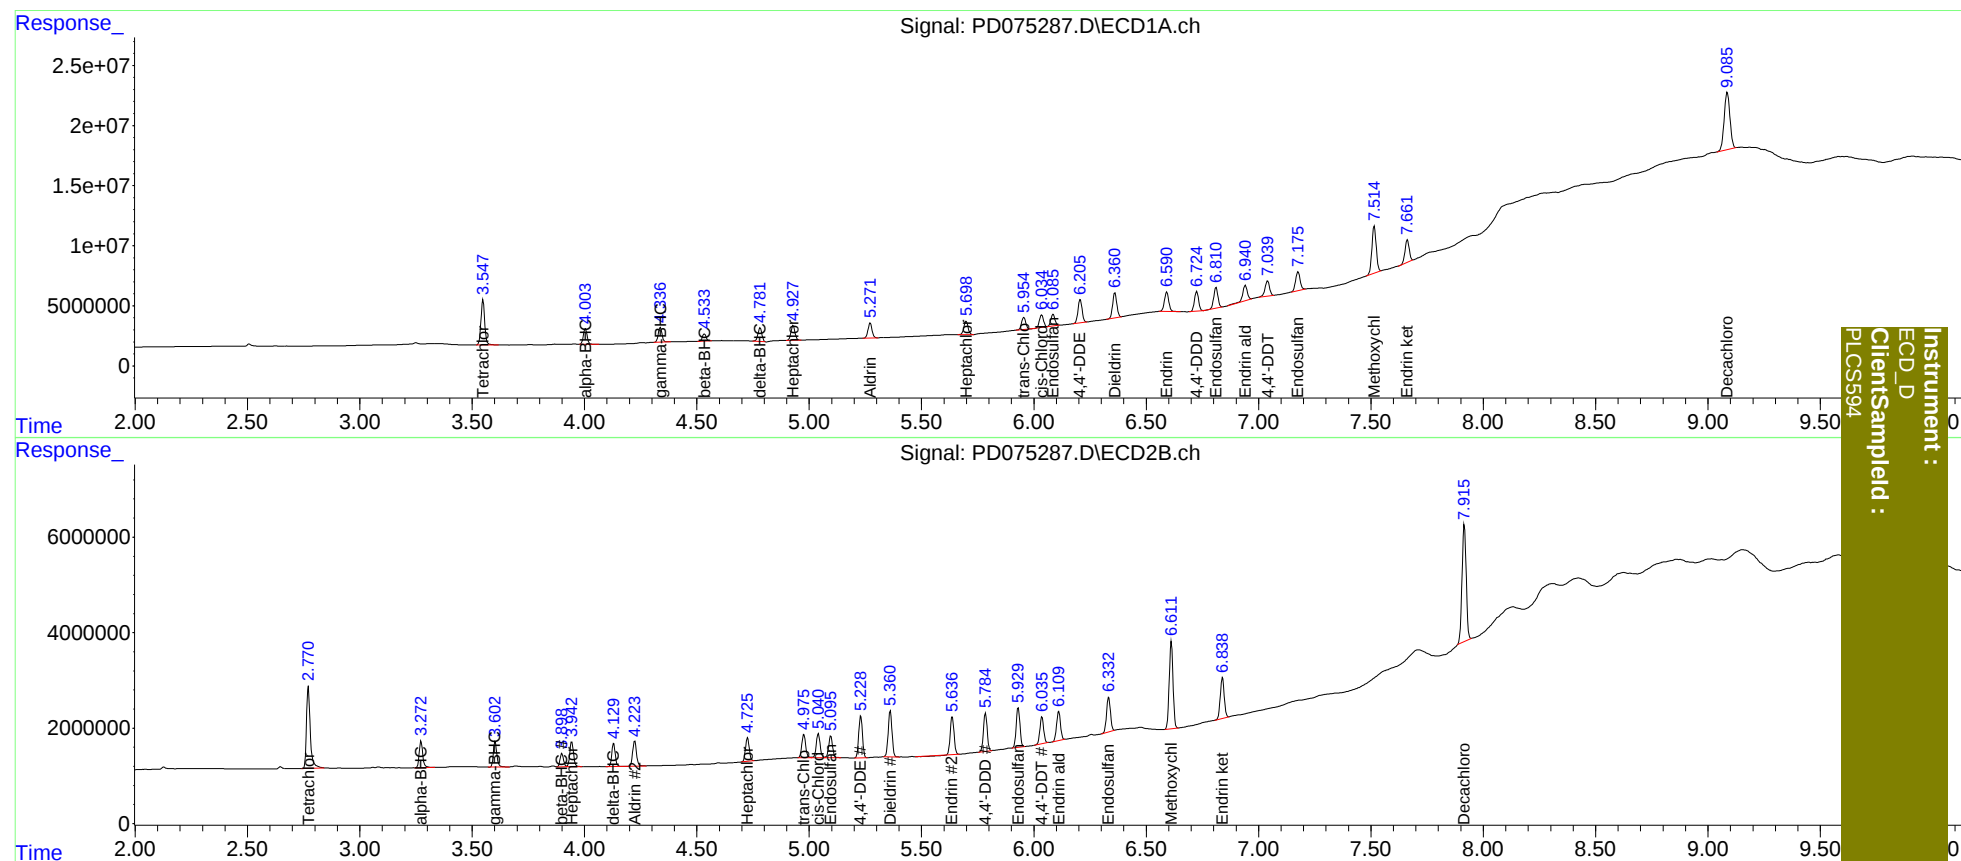

Instrument :
ECD_D
ClientSampled :
PLCS594