

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
 Data File : PD075290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 23:08
 Operator : AR\AJ
 Sample : 02589-03MSD
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JREA1MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/06/2023
 Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 00:28:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.549	2.772	42221571	19403006	18.511	18.396
27) SA Decachlor...	9.086	7.916	69077216	23182186	27.913	24.547
Target Compounds						
2) A alpha-BHC	4.005	3.274	202.0E6	76778305	52.515	49.566
3) MA gamma-BHC...	4.337	3.604	171.4E6	72318008	47.675m	49.198
4) MA Heptachlor	4.929	3.944	180.9E6	72387827	48.512	49.540
5) MB Aldrin	5.272	4.224	189.4E6	74515745	51.922	50.244
6) B beta-BHC	4.534	3.900	73308128	31670848	44.660	43.495
7) B delta-BHC	4.782	4.131	135.2E6	58842007	39.996	37.240
8) B Heptachlo...	5.699	4.727	162.9E6	63861965	48.059	45.787
9) A Endosulfan I	6.086	5.097	146.4E6	58320962	48.537	48.594
10) B trans-Chl...	5.956	4.977	159.2E6	69013880	48.598	50.576
11) B cis-Chlor...	6.035	5.041	176.5E6	66756253	51.782	47.834
12) B 4,4'-DDE	6.207	5.231	328.4E6	129.0E6	100.574	100.379
13) MA Dieldrin	6.361	5.362	355.8E6	136.6E6	104.044	100.140
14) MA Endrin	6.592	5.637	285.6E6	119.7E6	98.745	98.371
15) B Endosulfa...	6.811	5.932	281.2E6	111.5E6	87.309	87.166
16) A 4,4'-DDD	6.725	5.785	260.5E6	102.9E6	107.806	103.819
17) MA 4,4'-DDT	7.040	6.037	286.8E6	110.1E6	113.007	109.204
18) B Endrin al...	6.941	6.111	198.0E6	80871459	83.717	79.639
19) B Endosulfa...	7.177	6.334	251.5E6	98554063	91.435	84.739
20) A Methoxychlor	7.515	6.612	658.6E6	253.3E6	448.338	442.159
21) B Endrin ke...	7.663	6.840	311.5E6	118.1E6	102.778	89.563

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
Data File : PD075290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 23:08
Operator : AR\AJ
Sample : 02589-03MSD
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 00:28:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

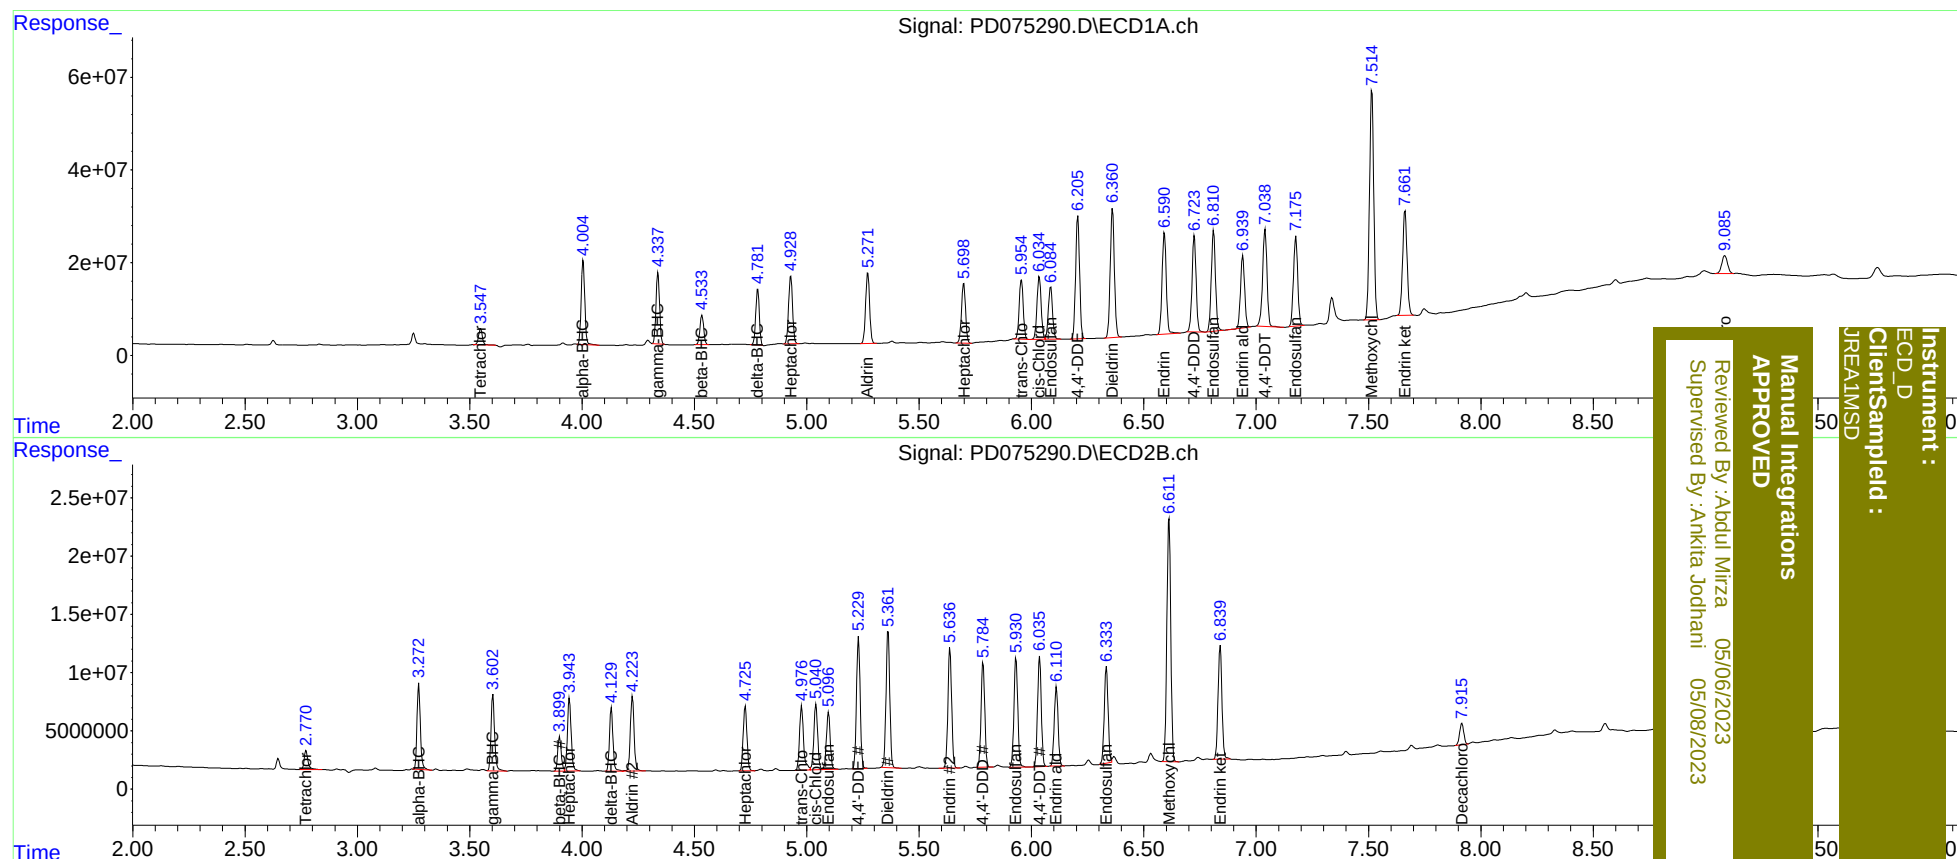

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Instrument :
ECD_D
Client Sampled :
JREALMSD