

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
 Data File : PD075289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2023 22:55
 Operator : AR\AJ
 Sample : 02589-02MS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JREA1MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/06/2023
 Supervised By :Ankita Jodhani 05/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 00:28:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.549	2.772	43459106	19521230	19.054	18.508
27) SA Decachlor...	9.087	7.915	68964980	23103047	27.868	24.464
Target Compounds						
2) A alpha-BHC	4.004	3.274	204.3E6	77380921	53.134	49.955
3) MA gamma-BHC...	4.336	3.604	172.5E6	72691619	47.988m	49.452
4) MA Heptachlor	4.929	3.944	182.5E6	72483848	48.951	49.606
5) MB Aldrin	5.272	4.224	191.8E6	75175583	52.588	50.688
6) B beta-BHC	4.534	3.900	73890634	31825820	45.014	43.708
7) B delta-BHC	4.782	4.131	136.7E6	59056757	40.442	37.375
8) B Heptachlo...	5.699	4.726	164.5E6	64289083	48.550	46.093
9) A Endosulfan I	6.086	5.097	147.6E6	58748786	48.923	48.951
10) B trans-Chl...	5.956	4.977	160.1E6	69452376	48.848	50.897
11) B cis-Chlor...	6.035	5.041	178.2E6	66991716	52.284	48.003
12) B 4,4'-DDE	6.207	5.230	331.2E6	129.6E6	101.419	100.792
13) MA Dieldrin	6.362	5.362	357.9E6	137.2E6	104.644	100.524
14) MA Endrin	6.592	5.637	285.6E6	119.8E6	98.773	98.496
15) B Endosulfa...	6.811	5.931	283.0E6	111.9E6	87.880	87.458
16) A 4,4'-DDD	6.725	5.785	263.1E6	103.7E6	108.886	104.604
17) MA 4,4'-DDT	7.040	6.036	283.4E6	110.2E6	111.669	109.377
18) B Endrin al...	6.941	6.110	201.9E6	81024437	85.367	79.790
19) B Endosulfa...	7.176	6.333	251.4E6	99794213	91.378	85.806
20) A Methoxychlor	7.515	6.612	662.6E6	252.8E6	451.047	441.388
21) B Endrin ke...	7.662	6.840	309.1E6	118.8E6	101.977	90.125

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050523\
Data File : PD075289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2023 22:55
Operator : AR\AJ
Sample : 02589-02MS
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 00:28:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

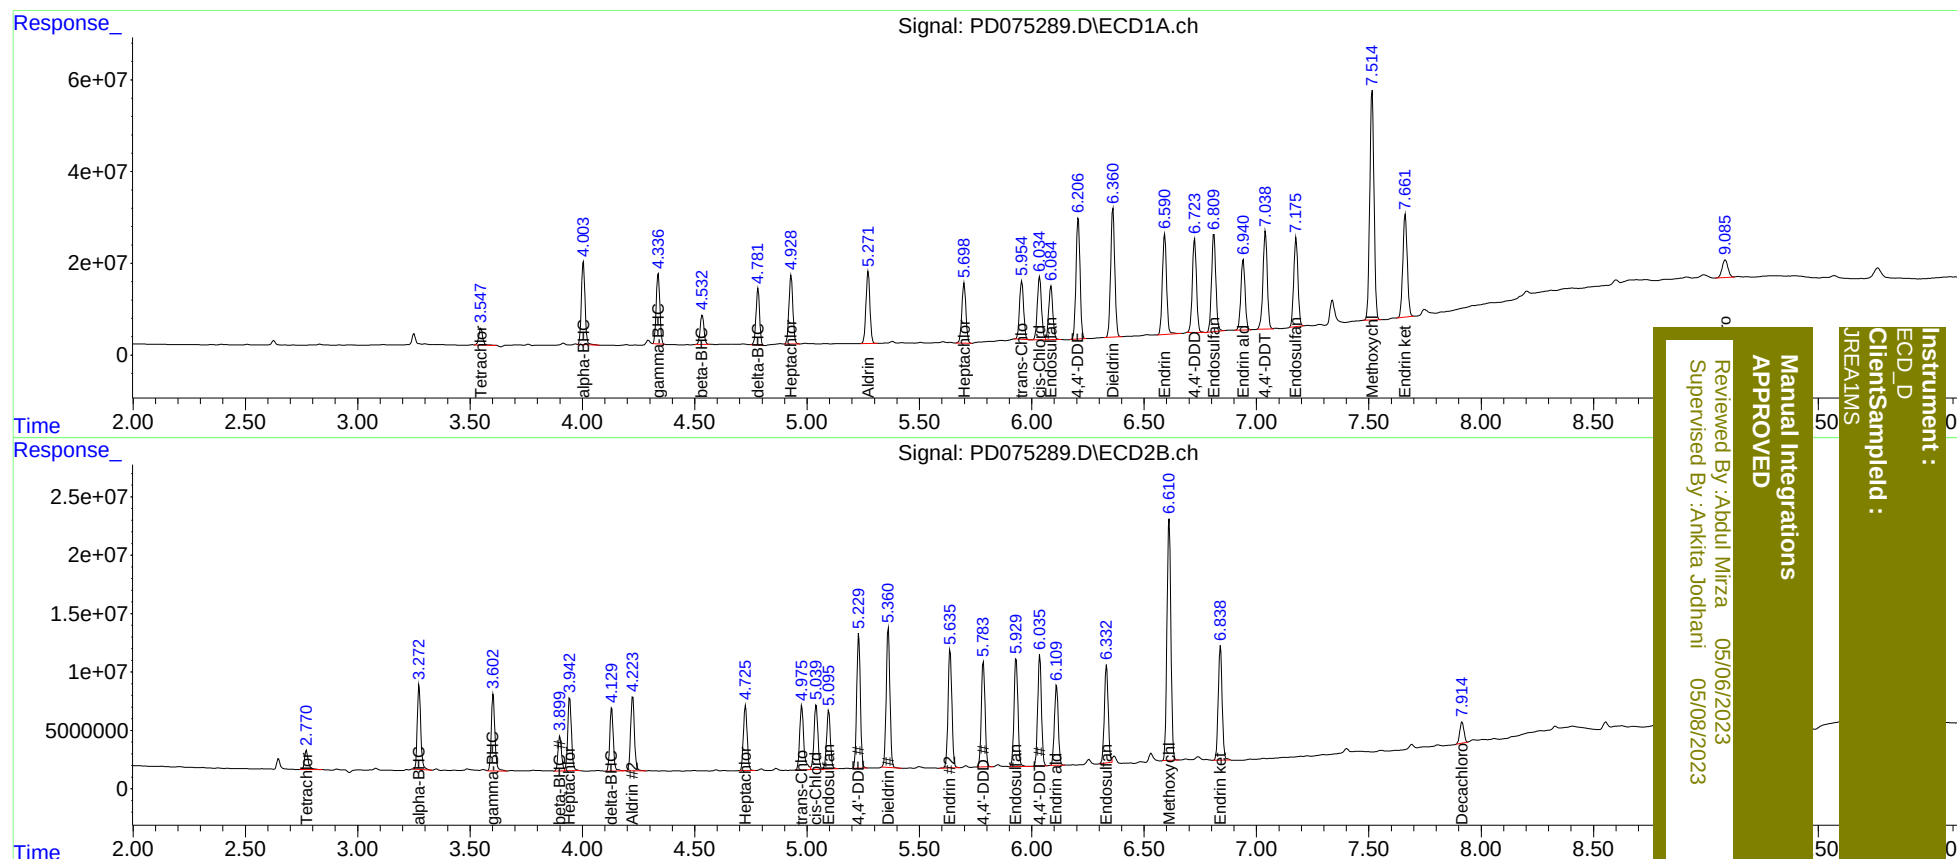

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 05/06/2023
Supervised By: Ankita Jodhani 05/08/2023

Instrument :
ECD_D
Client Sampled :
JREALMS