

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
 Data File : PD062725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 17:18
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 04:37:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 04:36:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.972	104.9E6	1104.6E6	96.402	92.519
28)	SA Decachlor...	8.203	9.033	104.9E6	1101.4E6	94.929	95.315
Target Compounds							
23)	Chlordane-1	4.311	4.965	33572728	538.9E6	944.795	932.346
24)	Chlordane-2	4.813	5.432	39230007	499.5E6	962.269	924.722
25)	Chlordane-3	5.383	6.078	117.9E6	2130.2E6	961.344	946.977
26)	Chlordane-4	5.441	6.153	98033944	2434.8E6	969.473	944.057
27)	Chlordane-5	6.279	6.957	43170885	482.7E6	971.928	979.064



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
Data File : PD062725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 17:18
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 04:37:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 04:36:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

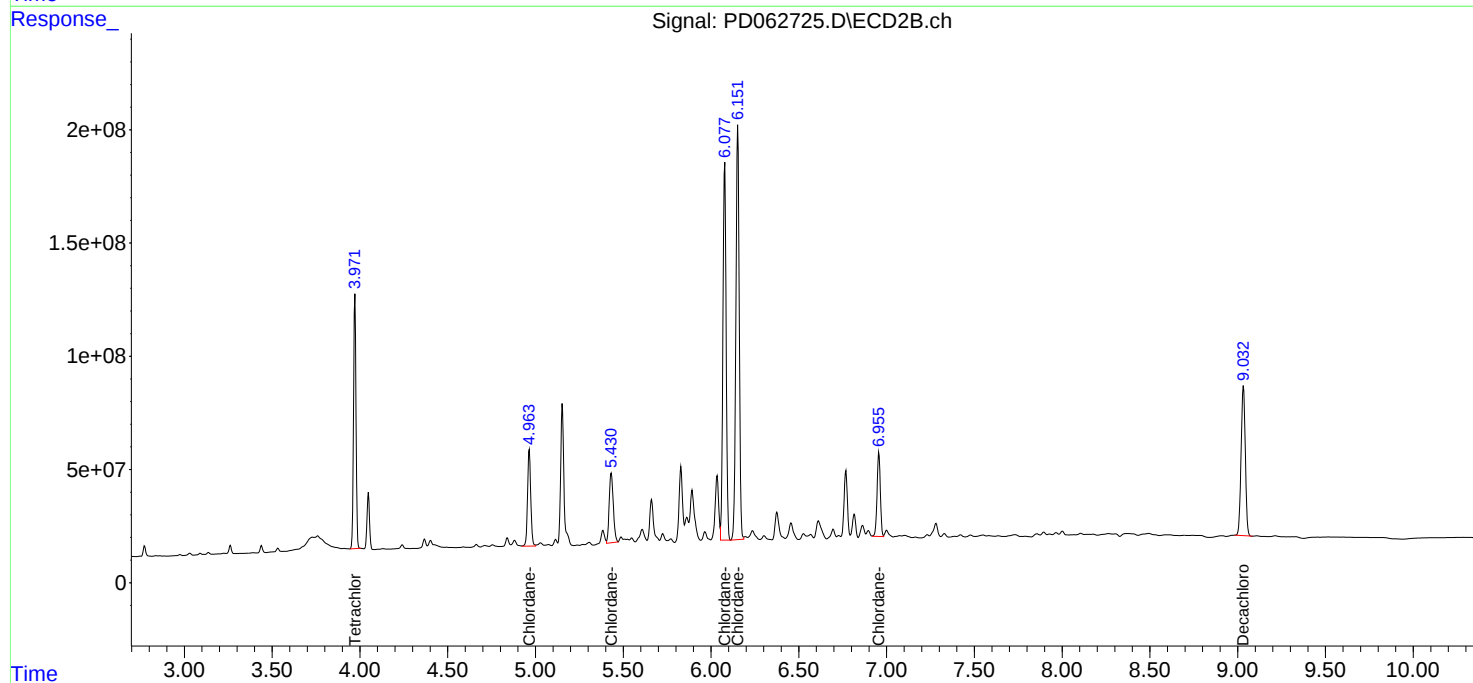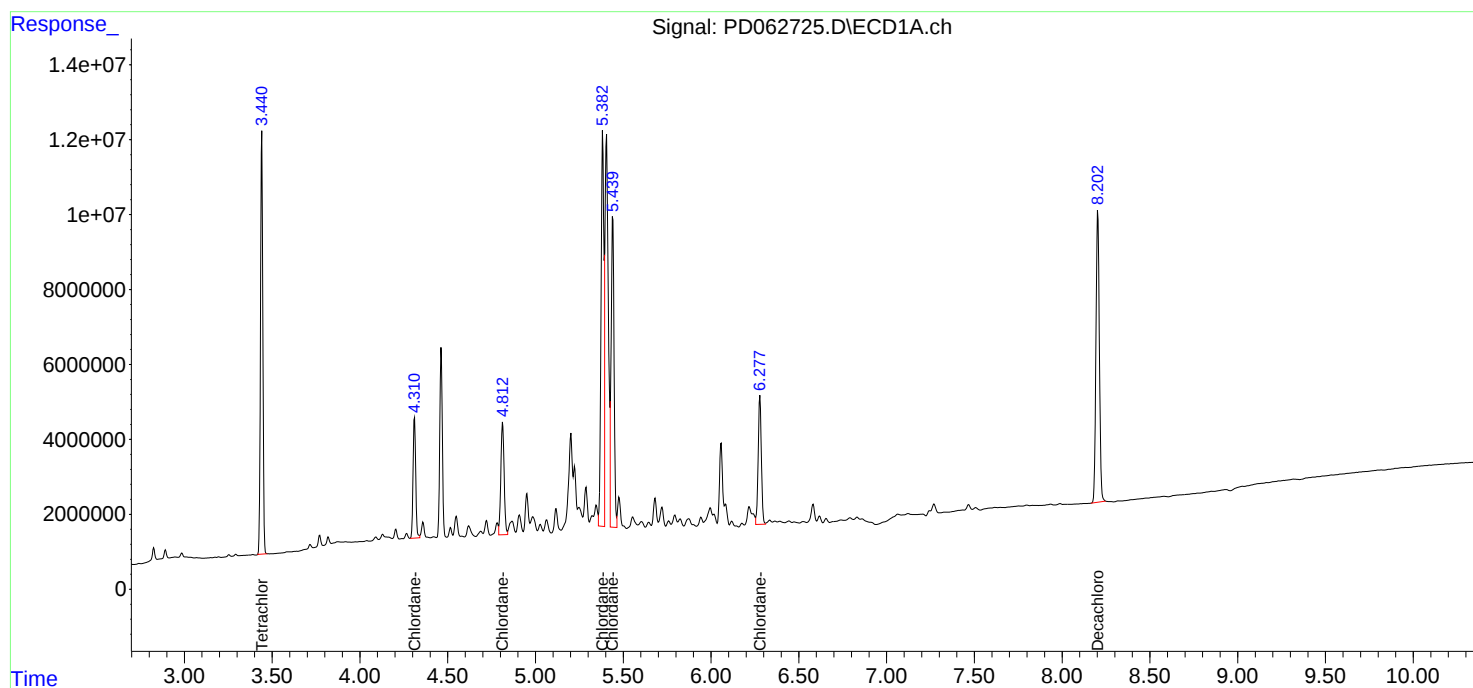


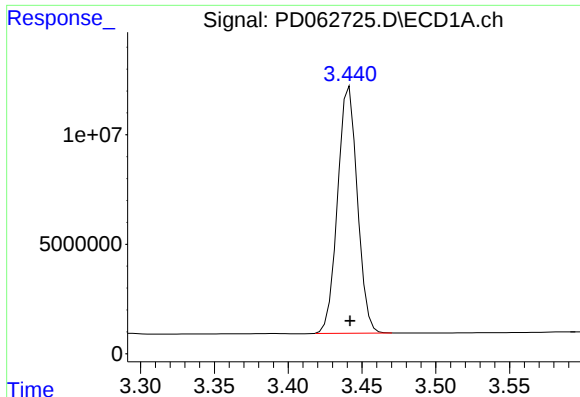

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 104913542
Conc: 96.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

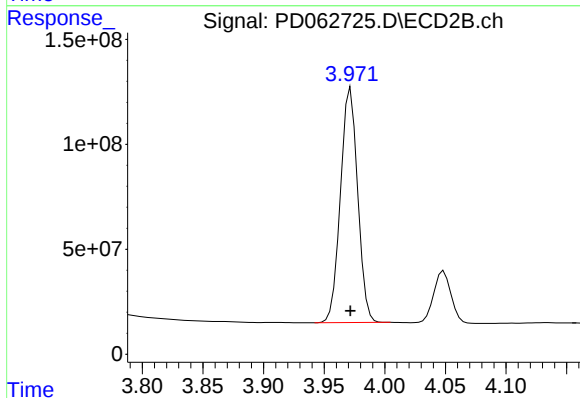


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.000 min
Response: 1104580150
Conc: 92.52 ng/ml

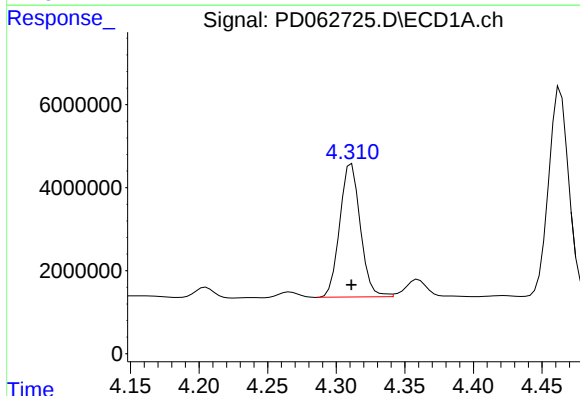


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 33572728
Conc: 944.79 ng/ml

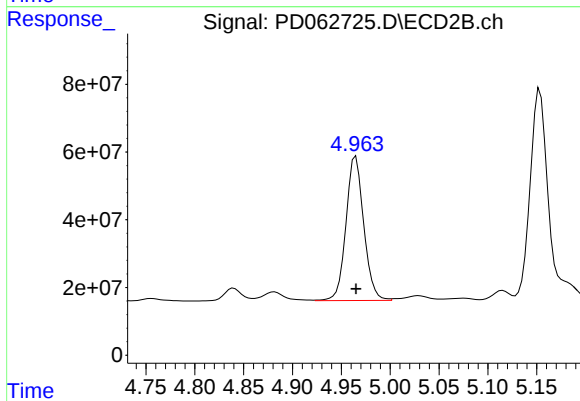

#23 Chlordane-1


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 538922108
Conc: 932.35 ng/ml

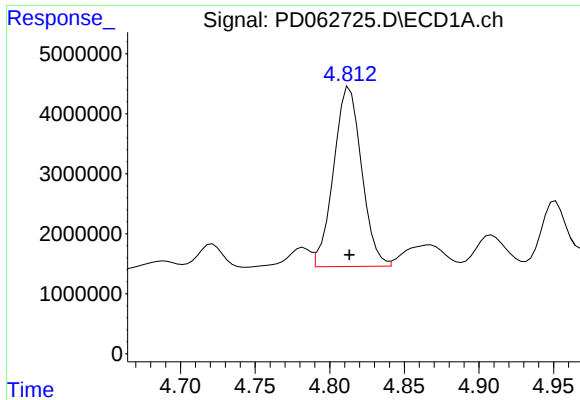

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 39230007
Conc: 962.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

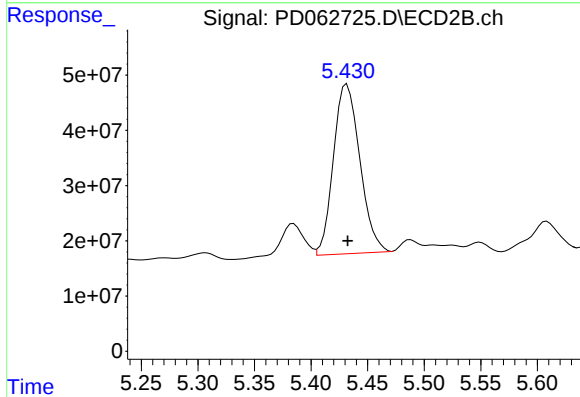


#24 Chlordane-2

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 499465411
Conc: 924.72 ng/ml

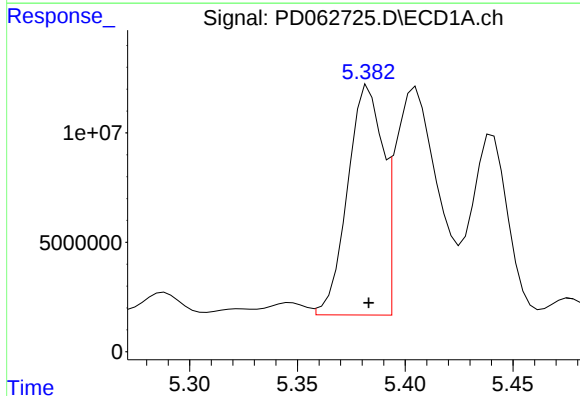


#25 Chlordane-3

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 117931037
Conc: 961.34 ng/ml

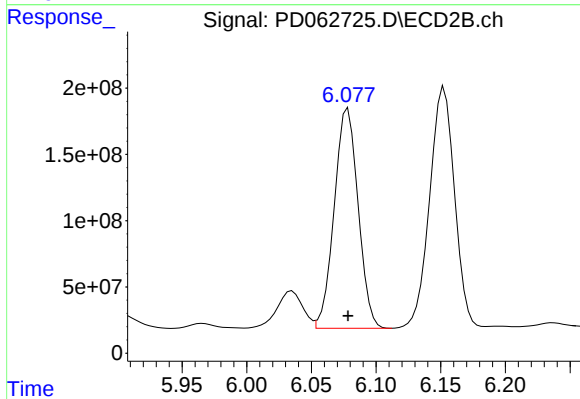

#25 Chlordane-3


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 2130177311
Conc: 946.98 ng/ml

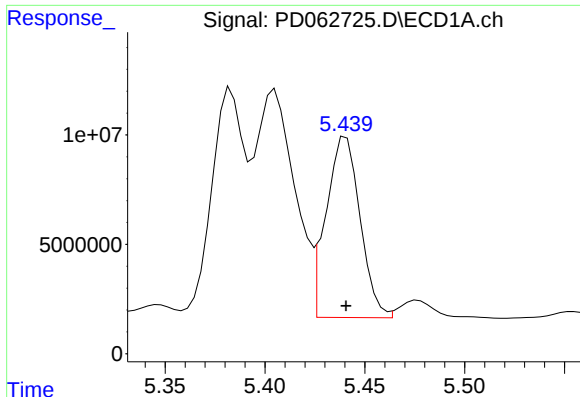

#26 Chlordane-4


R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 98033944
Conc: 969.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

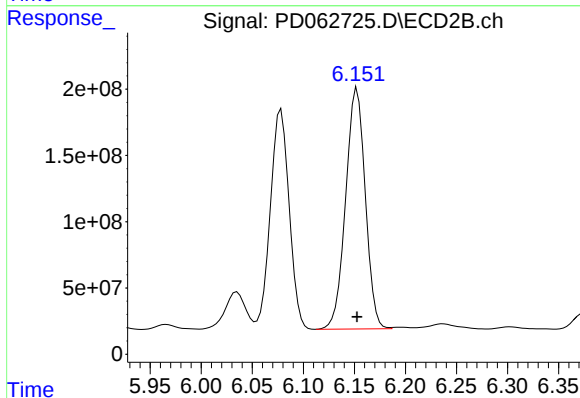


#26 Chlordane-4

R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 2434815931
Conc: 944.06 ng/ml

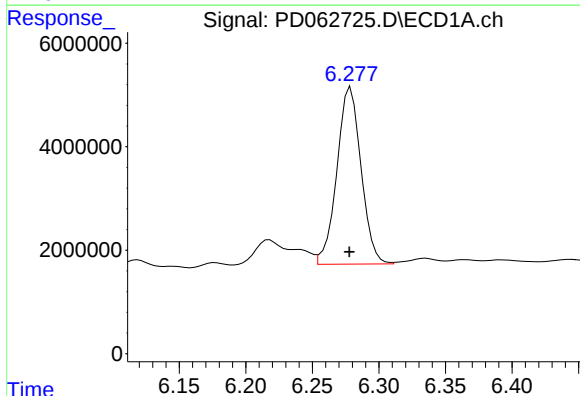


#27 Chlordane-5

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 43170885
Conc: 971.93 ng/ml

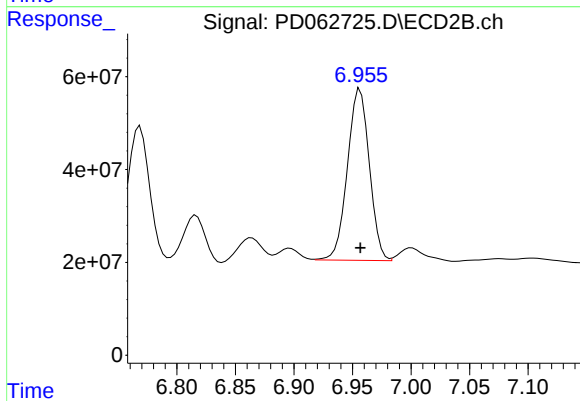

#27 Chlordane-5


R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 482687626
Conc: 979.06 ng/ml

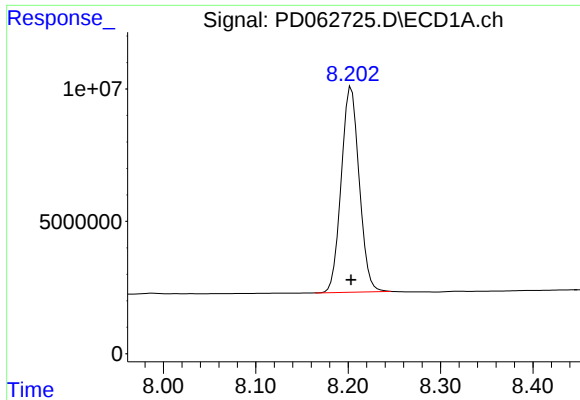

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.000 min
Response: 104903876
Conc: 94.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

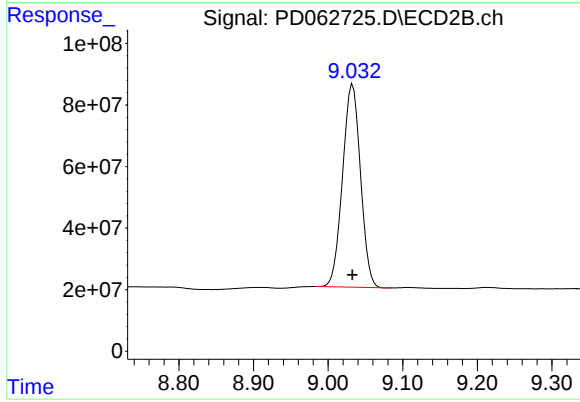

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.000 min
Response: 1101419124
Conc: 95.32 ng/ml