

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
 Data File : PD062736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 19:52
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD050621

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 04:48:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 04:47:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.972	53723610	585.8E6	50.982	49.550
28)	SA Decachlor...	8.203	9.031	55169539	590.2E6	51.285	51.618
Target Compounds							
23)	Chlordane-1	4.311	4.964	17621866	284.2E6	499.723	495.614
24)	Chlordane-2	4.813	5.432	20355695	267.3E6	499.796	500.730
25)	Chlordane-3	5.383	6.078	58870612	1111.4E6	496.818	497.279
26)	Chlordane-4	5.440	6.152	50479627	1279.6E6	520.543	496.105
27)	Chlordane-5	6.278	6.956	21764127	247.2E6	499.260	502.673



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
Data File : PD062736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 19:52
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD050621

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 04:48:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 04:47:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

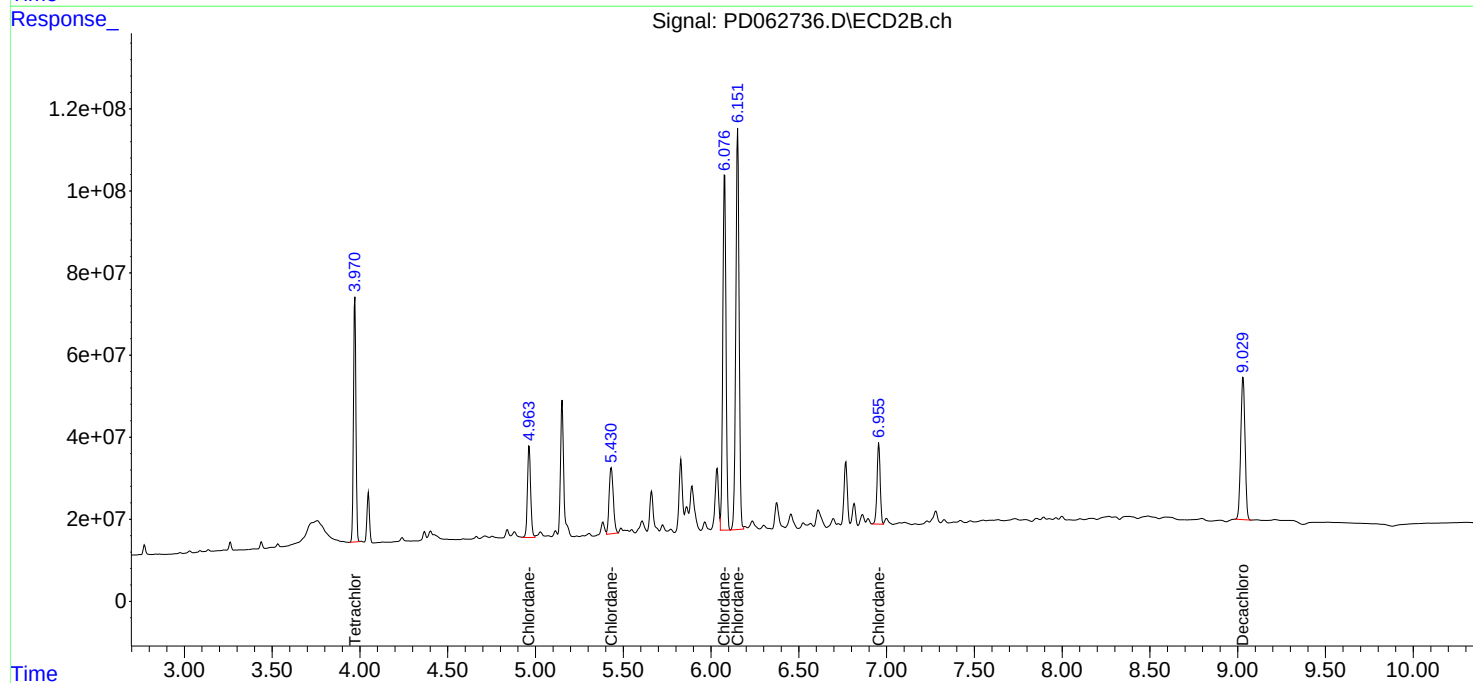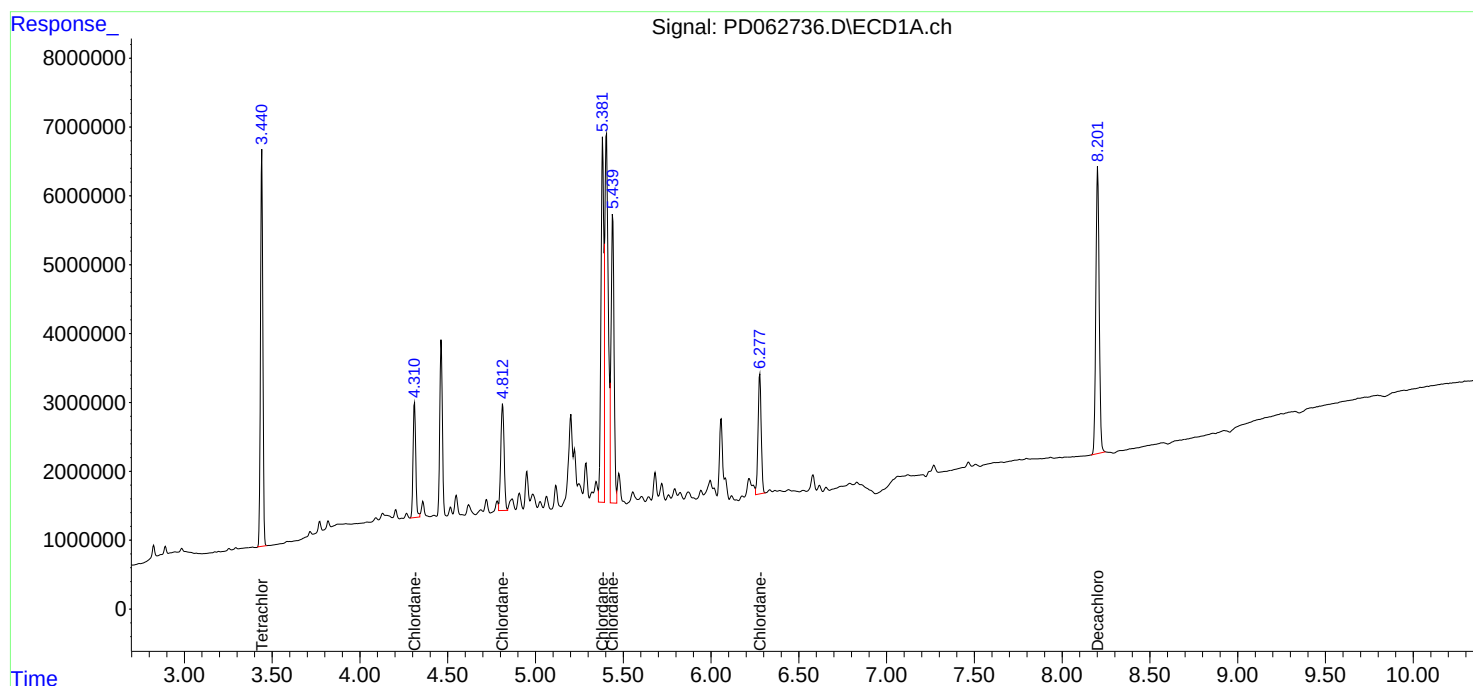


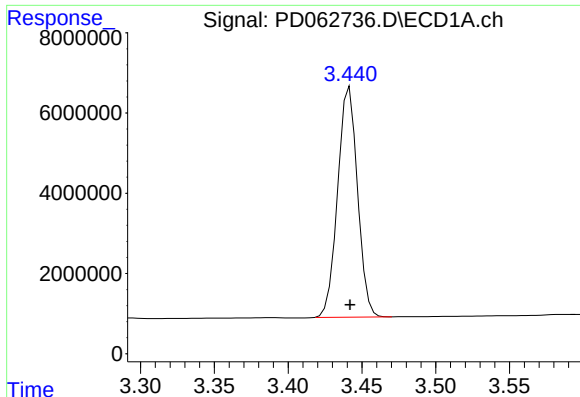

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 53723610
Conc: 50.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD050621

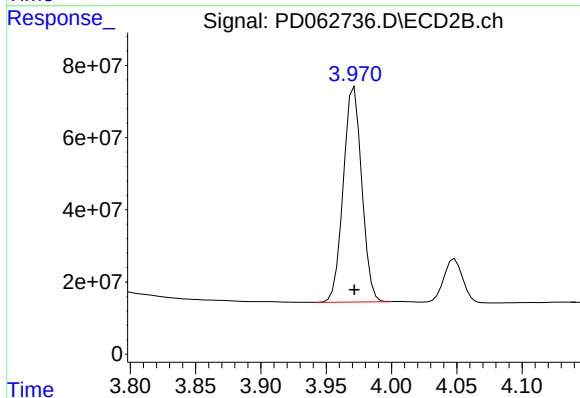


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.000 min
Response: 585768221
Conc: 49.55 ng/ml

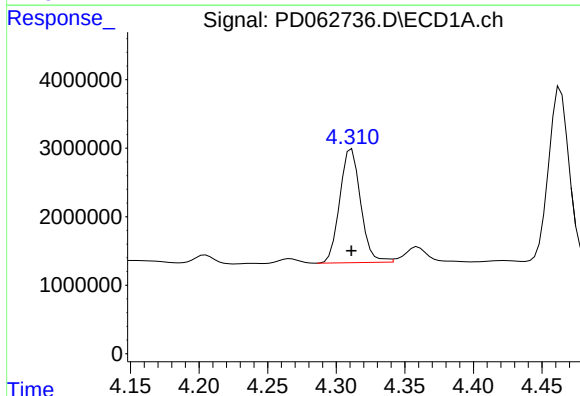


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 17621866
Conc: 499.72 ng/ml

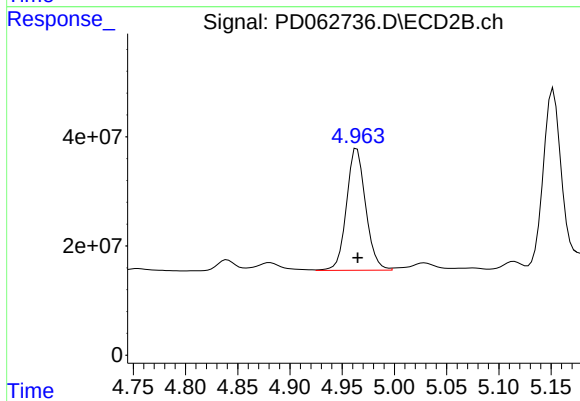

#23 Chlordane-1


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 284196981
Conc: 495.61 ng/ml

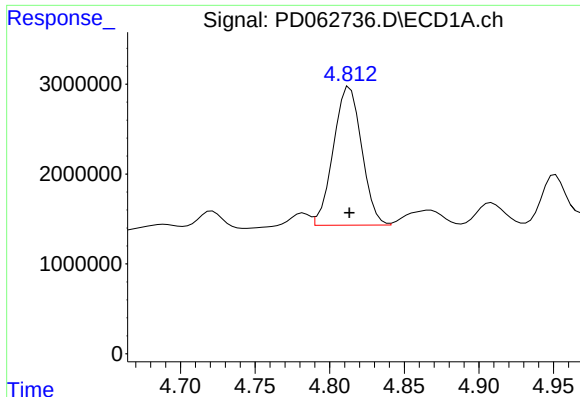

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 20355695
Conc: 499.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD050621

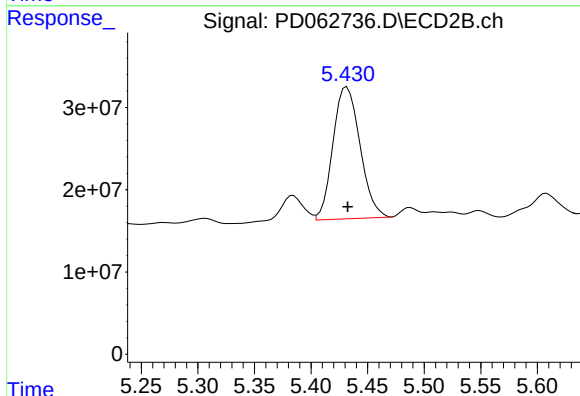


#24 Chlordane-2

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 267324407
Conc: 500.73 ng/ml

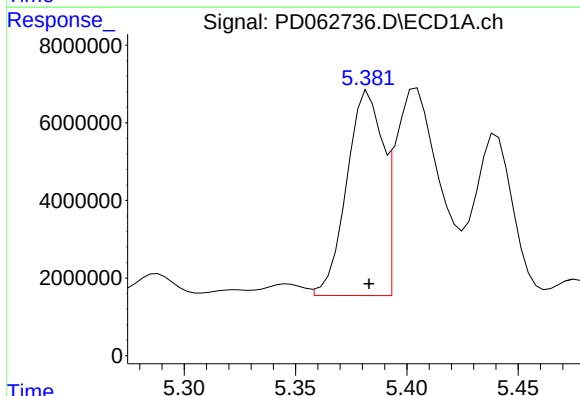


#25 Chlordane-3

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 58870612
Conc: 496.82 ng/ml

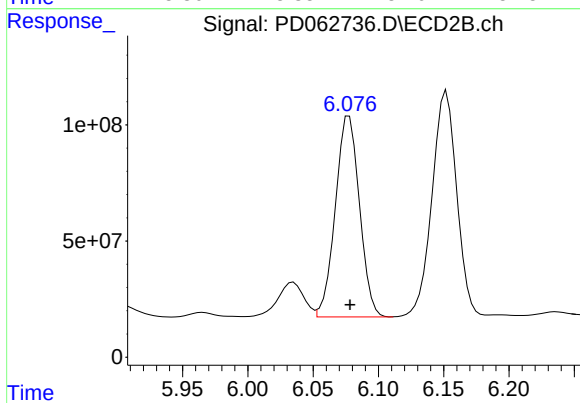

#25 Chlordane-3


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 1111374264
Conc: 497.28 ng/ml

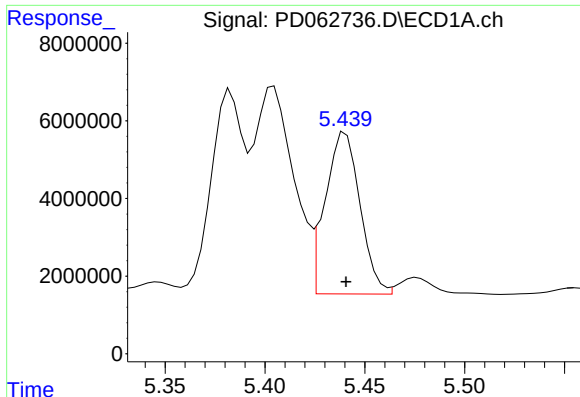

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 50479627
Conc: 520.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD050621

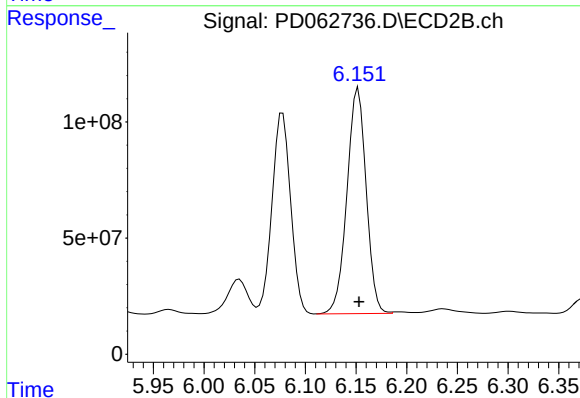


#26 Chlordane-4

R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 1279599950
Conc: 496.10 ng/ml

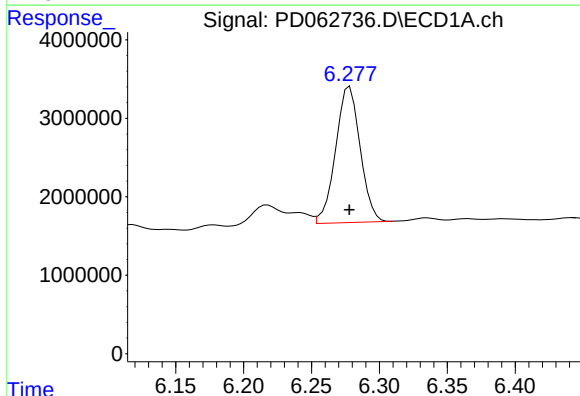


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 21764127
Conc: 499.26 ng/ml

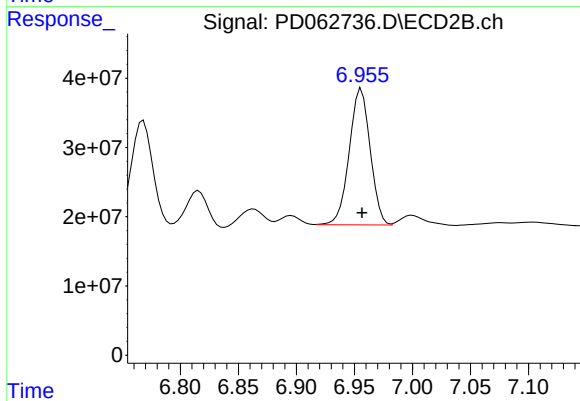

#27 Chlordane-5

R.T.: 6.956 min
Delta R.T.: 0.000 min
Response: 247236442
Conc: 502.67 ng/ml

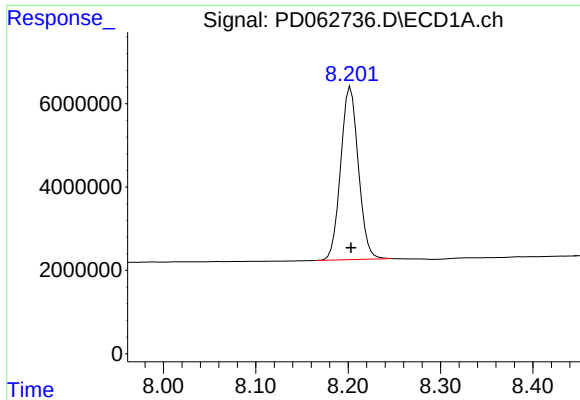

#28 Decachlorobiphenyl


R.T.: 8.203 min

Delta R.T.: 0.000 min

Response: 55169539

Conc: 51.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD050621

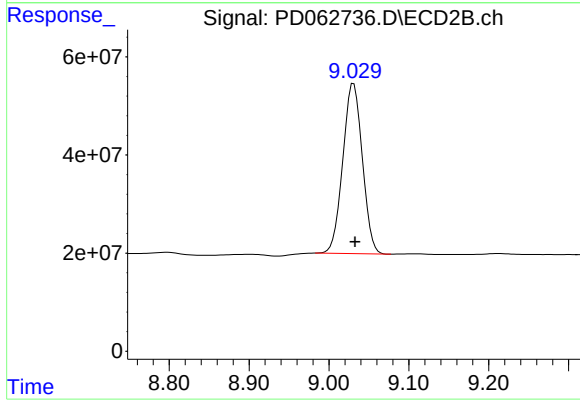

#28 Decachlorobiphenyl

R.T.: 9.031 min

Delta R.T.: -0.002 min

Response: 590165793

Conc: 51.62 ng/ml