

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
 Data File : PD062734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 19:24
 Operator : AR\AJ
 Sample : PTOXICC100
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC100

Manual Integrations
 APPROVED

Ankita
 5/6/2021 4:16:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 11:02:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 11:01:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.442	3.971	9194231	123.0E6	9.780	10.074
7) SA Decachlor...	8.203	9.031	10797519	117.8E6	9.472	9.923
Target Compounds						
2) Toxaphene-1	5.699	6.548	806603	13787988	105.366m	89.872
3) Toxaphene-2	6.184	7.055	775247	11352750	92.663	88.135
4) Toxaphene-3	6.301	7.130	1811830	36933779	93.466	102.006
5) Toxaphene-4	6.550	7.217	1814343	21255433	89.498	93.990
6) Toxaphene-5	7.038	7.630	2172589	14811362	98.238	90.308

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
Data File : PD062734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 19:24
Operator : AR\AJ
Sample : PTOXICC100
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 11:02:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 11:01:32 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

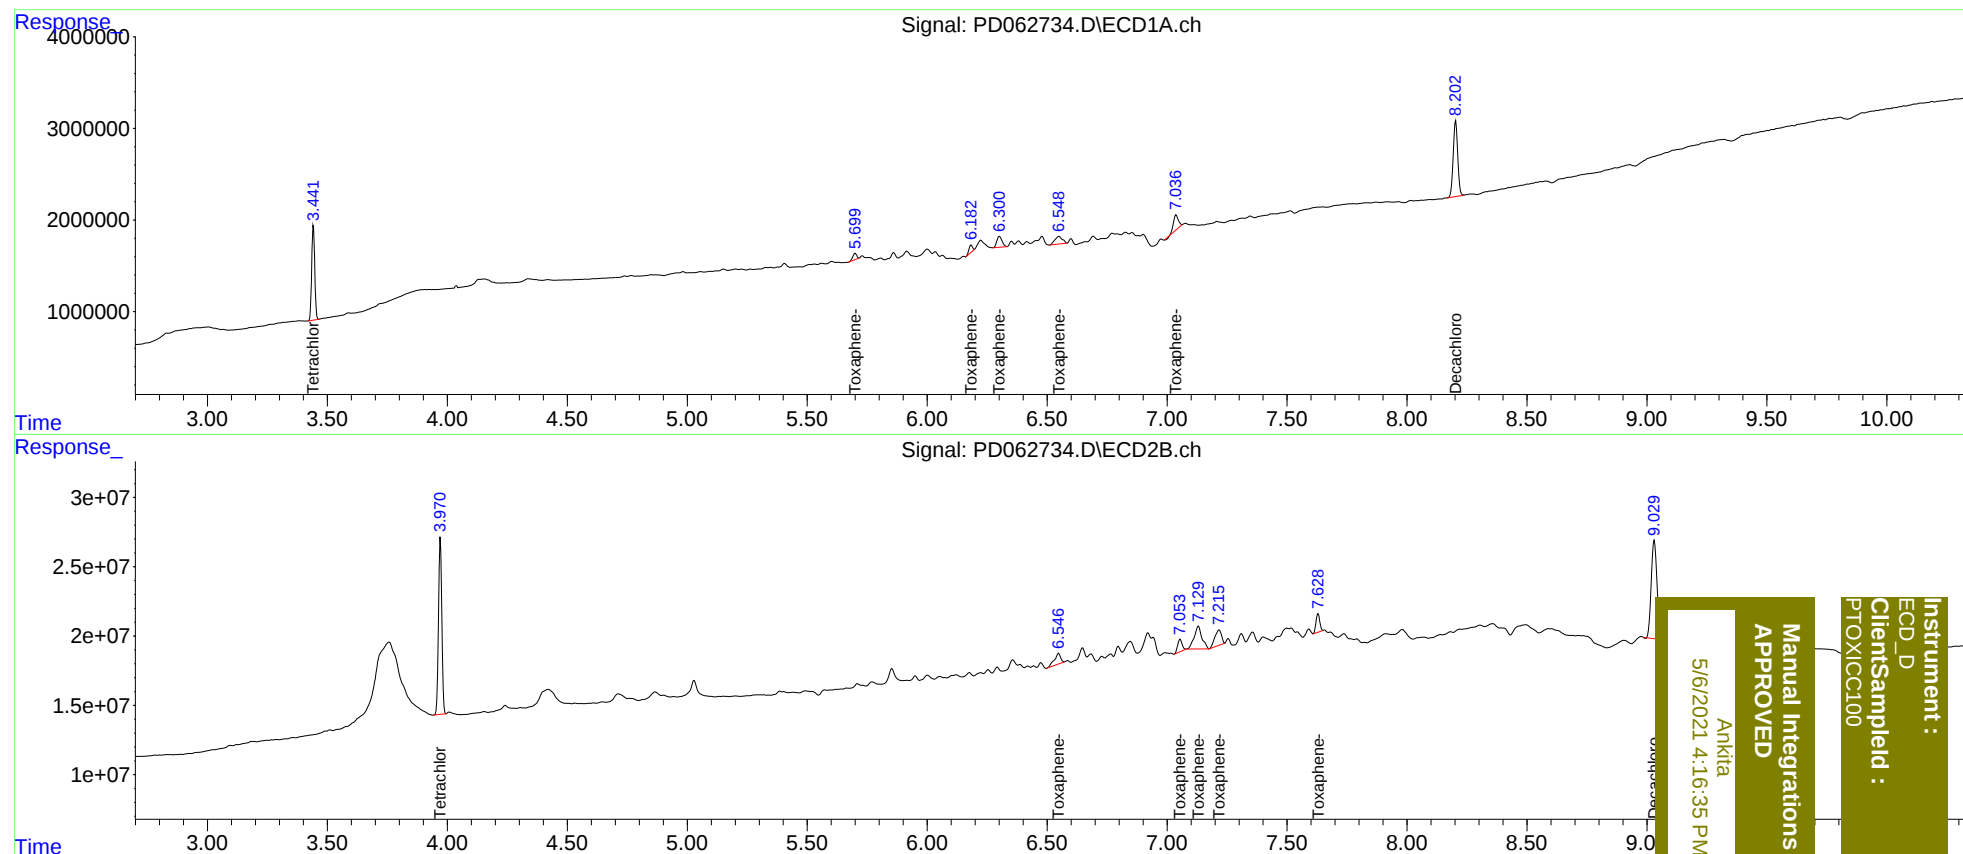

Manual Integrations
APPROVED

Ankita
5/6/2021 4:16:35 PM

Instrument :
ECD_D
ClientSampled :
PTOXICC100