

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
 Data File : PD062754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2021 00:03
 Operator : AR\AJ
 Sample : M2214-21
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-TXP-SOIL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 11:06:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 11:04:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.442	3.971	17226854	213.9E6	18.411	17.624
7) SA Decachlor...	8.202	9.031	20444764	229.7E6	18.261	19.396
Target Compounds						
2) Toxaphene-1	5.698	6.547	18839197	330.1E6	2447.317	2217.435
3) Toxaphene-2	6.182	7.053	20847642	289.6E6	2506.792	2326.013
4) Toxaphene-3	6.303	7.130	49532675	826.0E6	2608.578	2287.677
5) Toxaphene-4	6.548	7.216	50681516	525.2E6	2591.002	2348.196
6) Toxaphene-5	7.036	7.630	55715217	361.4E6	2514.943	2282.764

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
Data File : PD062754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2021 00:03
Operator : AR\AJ
Sample : M2214-21
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 11:06:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 11:04:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

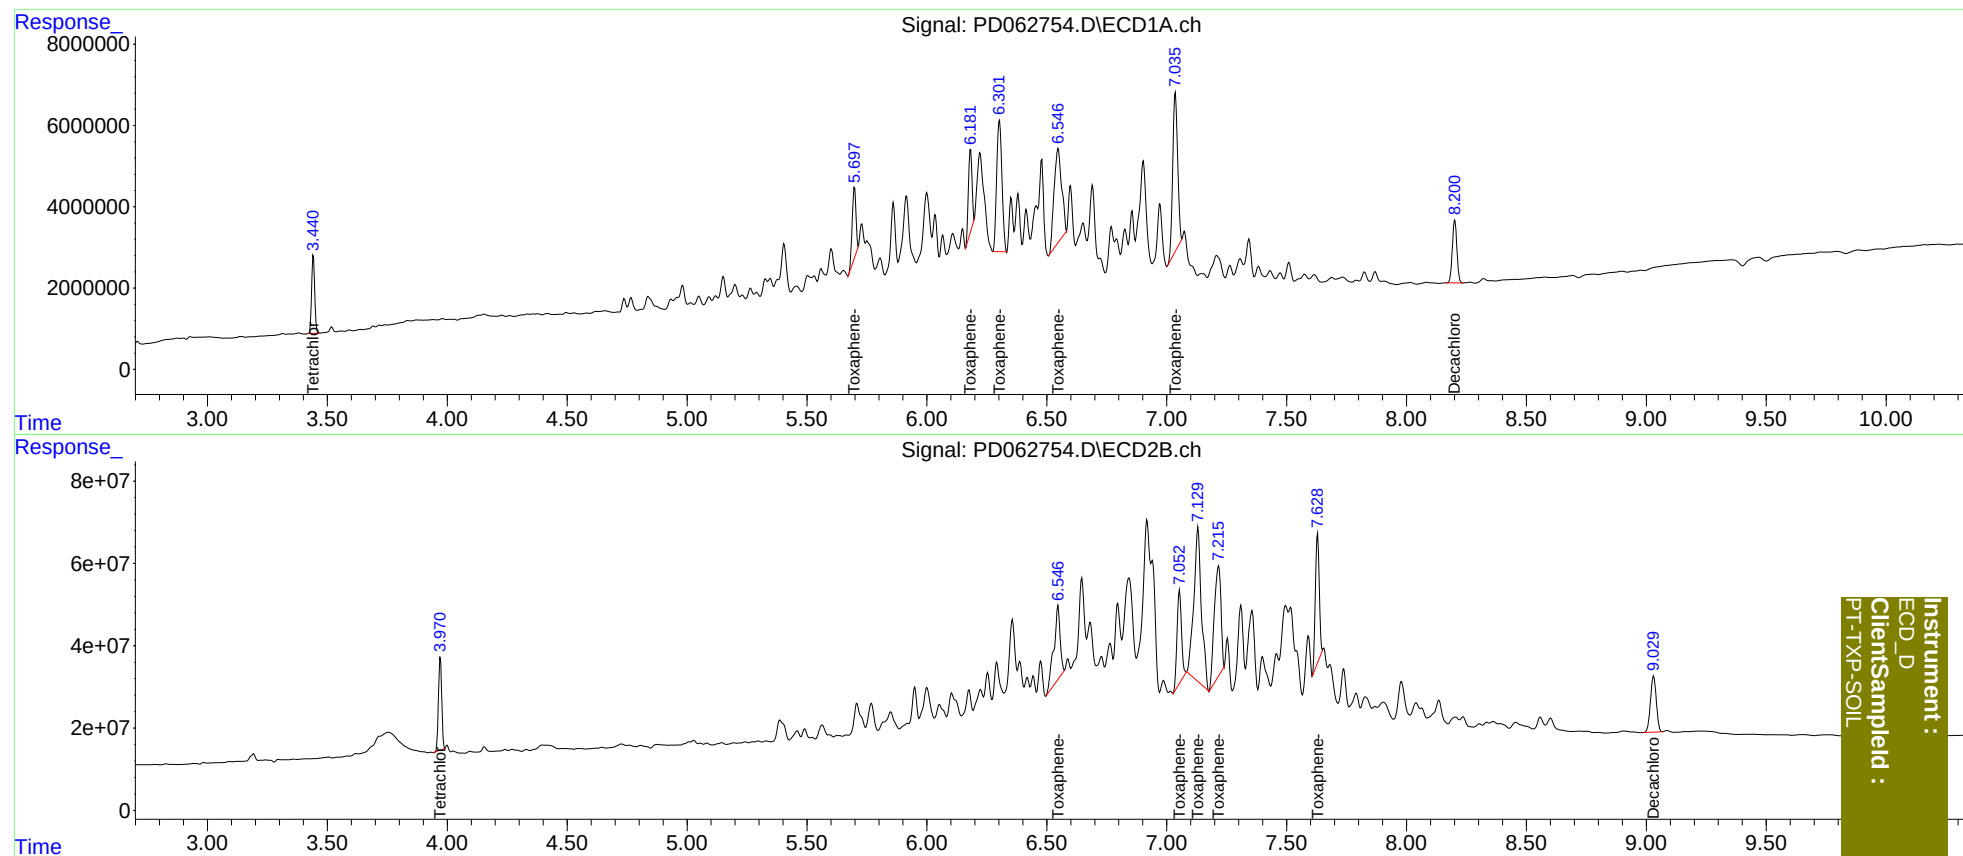

Instrument :
ECD_D
Client Sampled :
PT-TXP-SOIL