

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
 Data File : PD062726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 17:32
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 04:37:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 04:36:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	81481365	869.3E6	74.871	72.810
28)	SA Decachlor...	8.203	9.032	79698615	856.6E6	72.121	74.130
Target Compounds							
23)	Chlordane-1	4.312	4.964	26026521	422.7E6	732.431	731.362
24)	Chlordane-2	4.813	5.431	30825923	393.7E6	756.126	728.884
25)	Chlordane-3	5.383	6.078	90687336	1656.6E6	739.260	736.464
26)	Chlordane-4	5.441	6.153	75493026	1892.8E6	746.563	733.887
27)	Chlordane-5	6.278	6.956	32939749	369.9E6	741.589	750.264



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
Data File : PD062726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 17:32
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 04:37:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 04:36:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

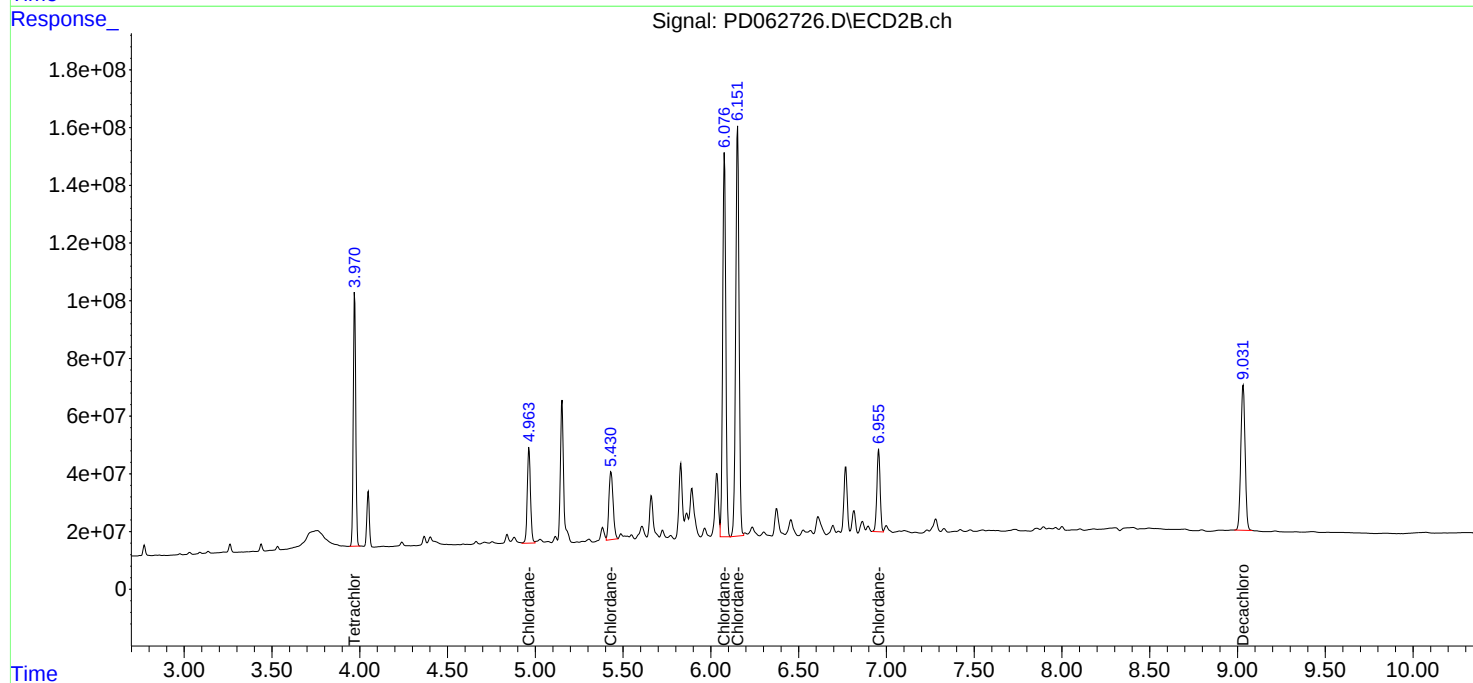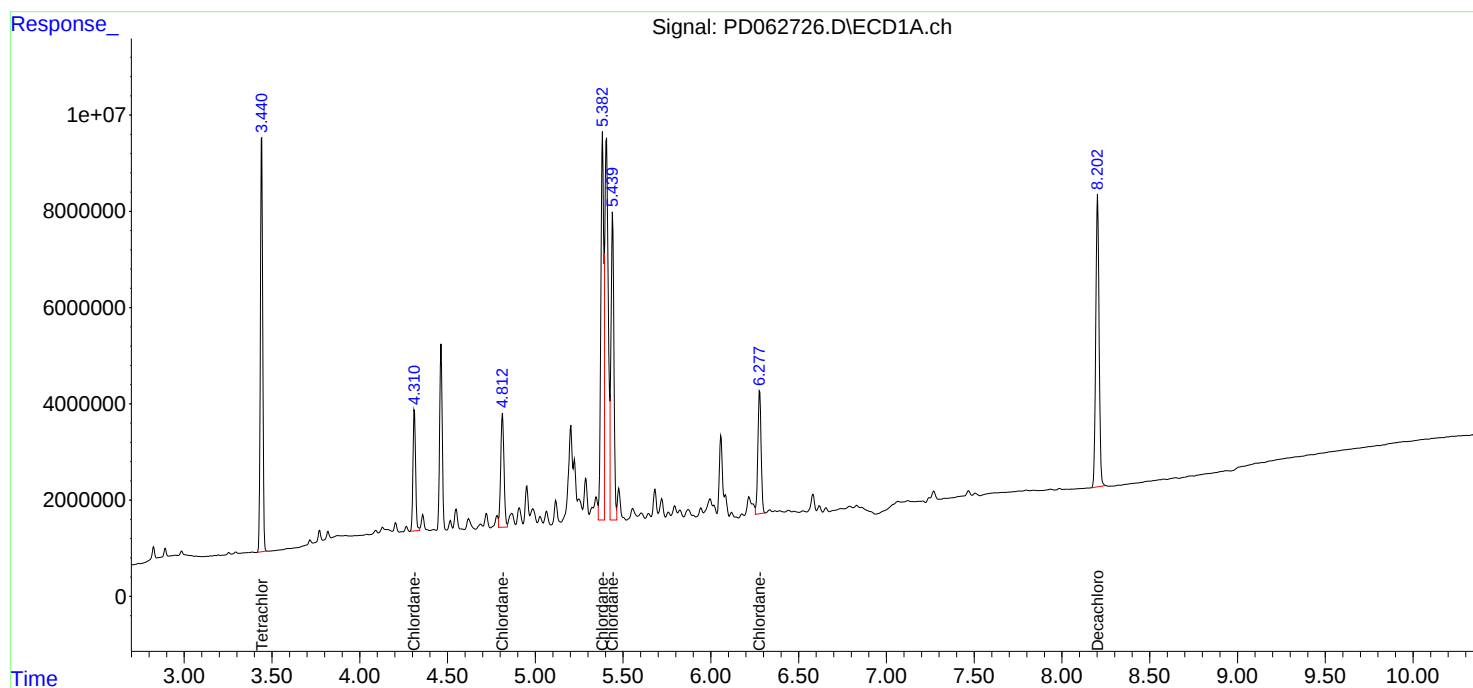


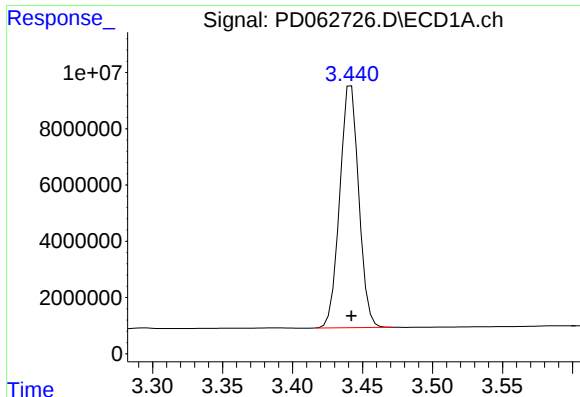

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 81481365
Conc: 74.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

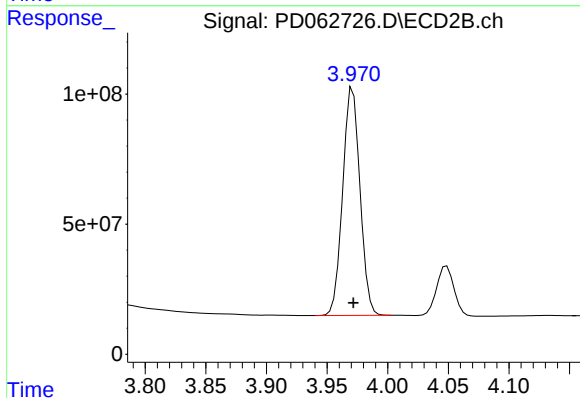


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 869276712
Conc: 72.81 ng/ml

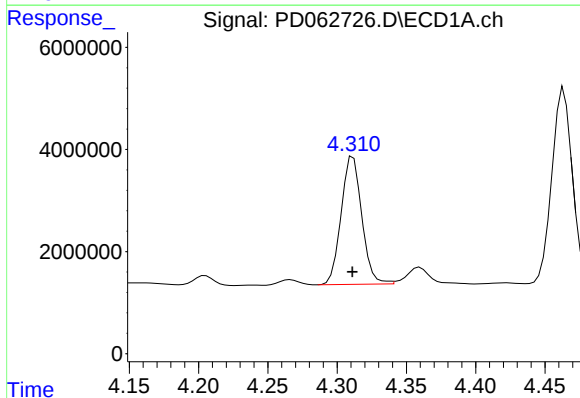


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 26026521
Conc: 732.43 ng/ml

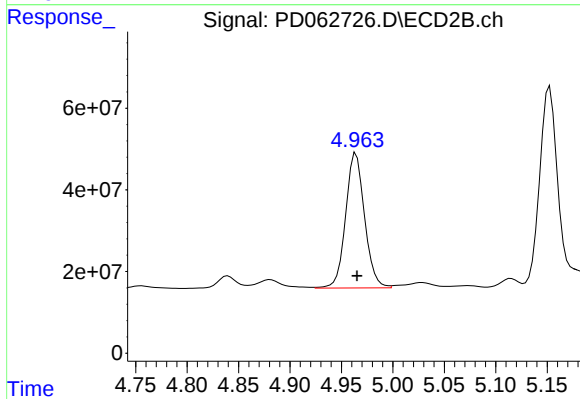

#23 Chlordane-1


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 422747264
Conc: 731.36 ng/ml

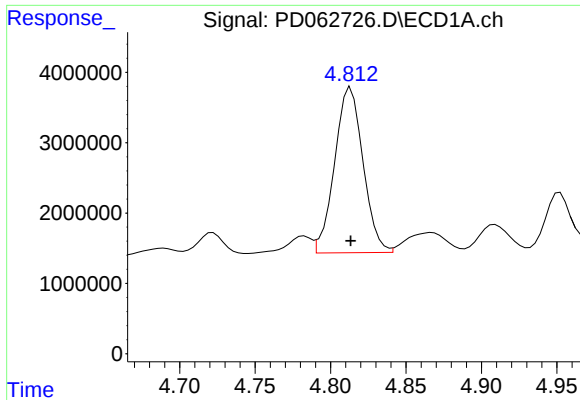

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 30825923
Conc: 756.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

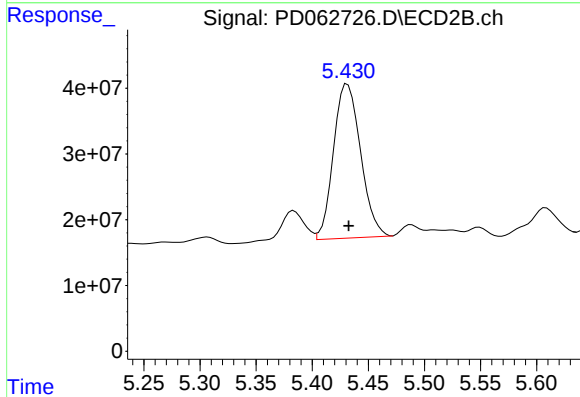


#24 Chlordane-2

R.T.: 5.431 min
Delta R.T.: -0.001 min
Response: 393688516
Conc: 728.88 ng/ml

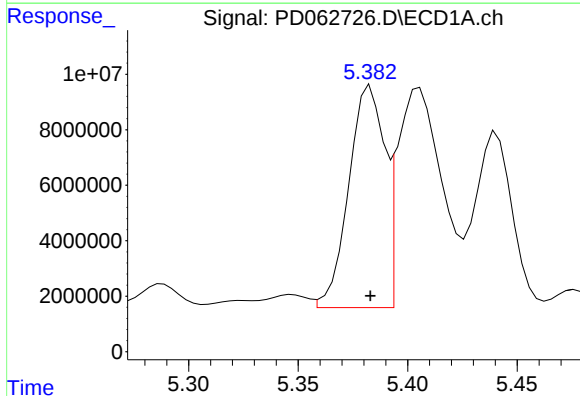


#25 Chlordane-3

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 90687336
Conc: 739.26 ng/ml

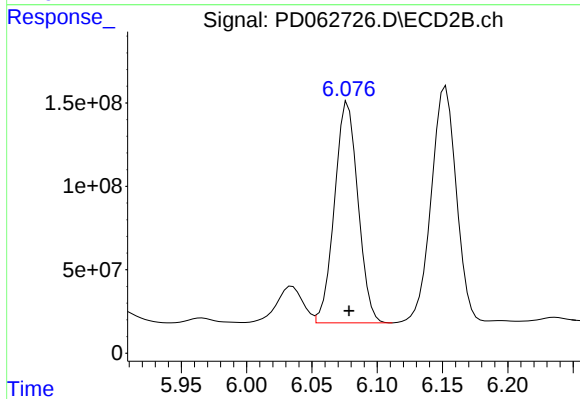

#25 Chlordane-3


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 1656638875
Conc: 736.46 ng/ml

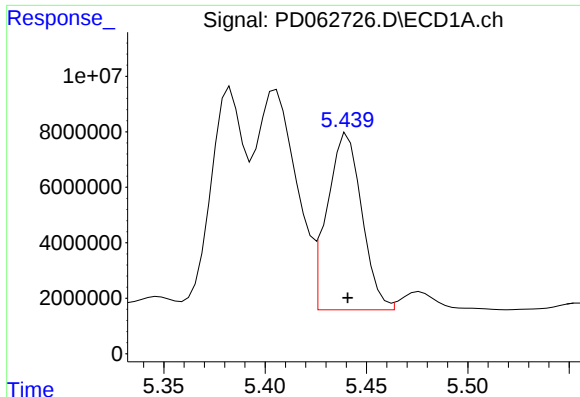

#26 Chlordane-4


R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 75493026
Conc: 746.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

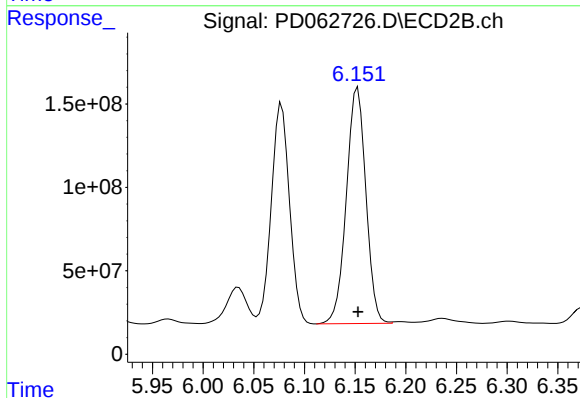


#26 Chlordane-4

R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 1892766605
Conc: 733.89 ng/ml

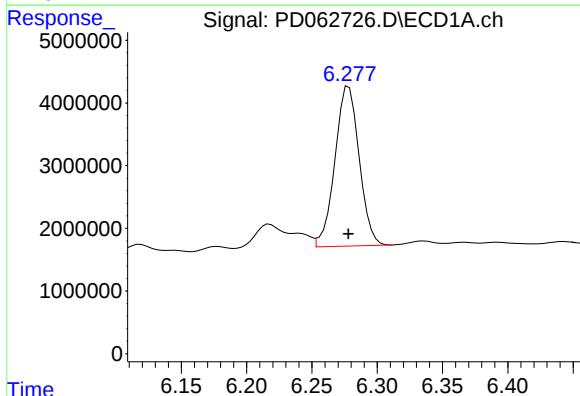


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 32939749
Conc: 741.59 ng/ml

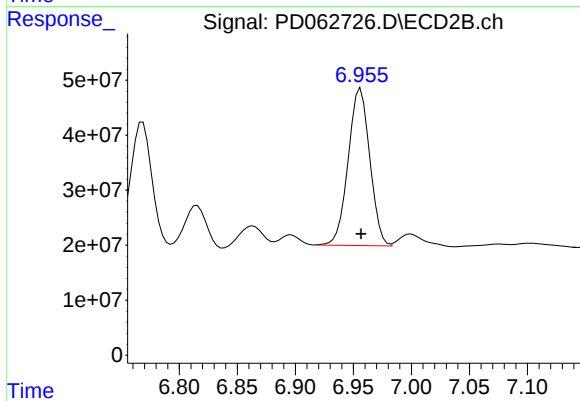

#27 Chlordane-5


R.T.: 6.956 min
Delta R.T.: 0.000 min
Response: 369887043
Conc: 750.26 ng/ml

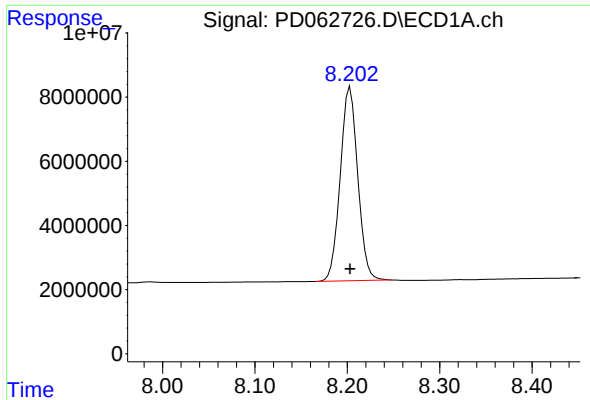

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.000 min
Response: 79698615
Conc: 72.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

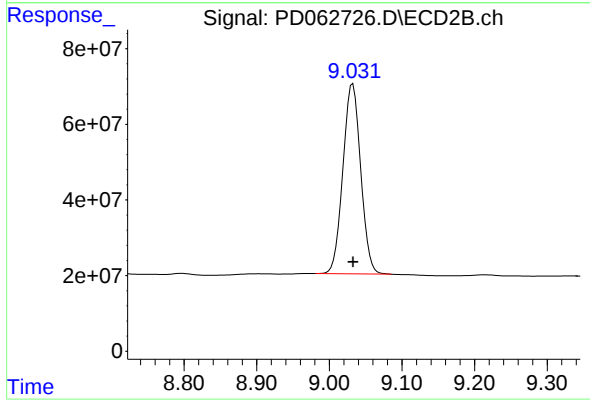

#28 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.000 min
Response: 856609140
Conc: 74.13 ng/ml