

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
 Data File : PD062728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 18:00
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 04:38:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 04:36:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.972	25758502	299.5E6	23.669	25.085
28)	SA Decachlor...	8.202	9.032	27354214	287.9E6	24.753	24.914
Target Compounds							
23)	Chlordane-1	4.311	4.965	8267126	148.2E6	232.651	256.452
24)	Chlordane-2	4.813	5.432	10205918	136.9E6	250.340	253.425
25)	Chlordane-3	5.382	6.078	27824811	565.4E6	226.821	251.329
26)	Chlordane-4	5.440	6.152	22736335	652.2E6	224.843	252.895
27)	Chlordane-5	6.278	6.956	11002243	125.2E6	247.699	253.862



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
Data File : PD062728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 18:00
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 04:38:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 04:36:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

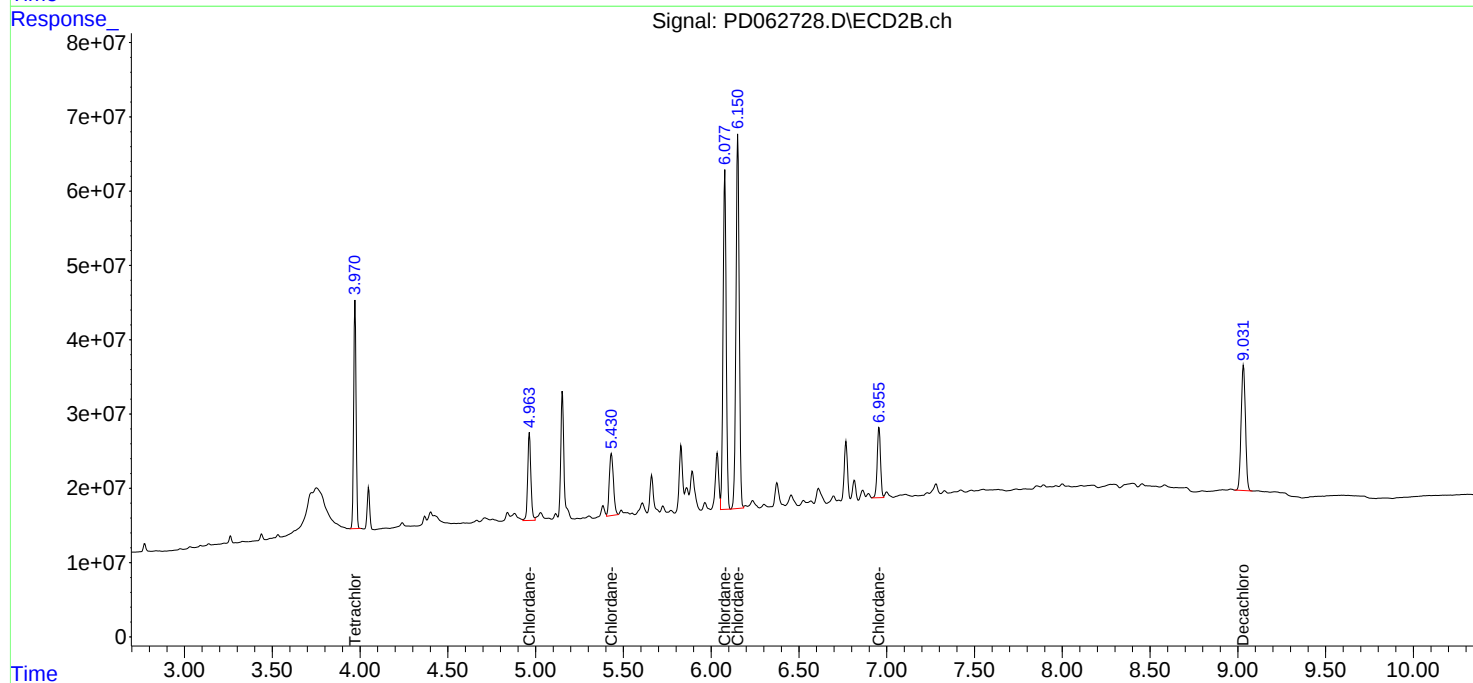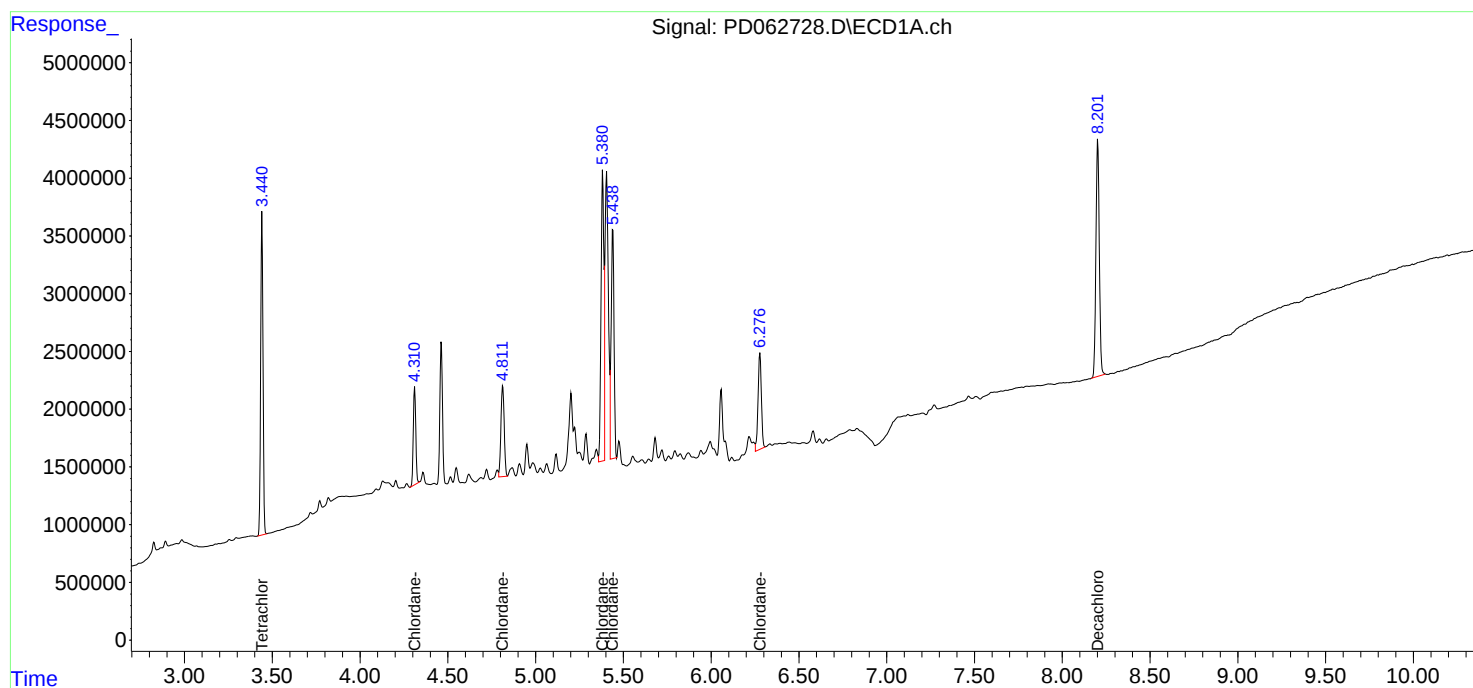


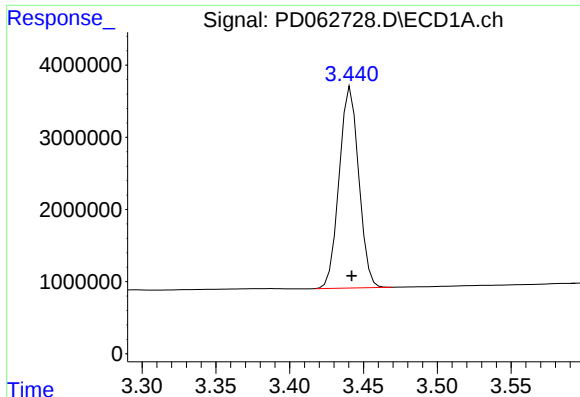

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 25758502
Conc: 23.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

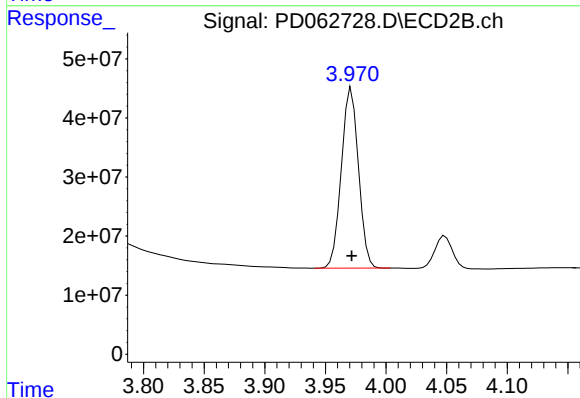


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: 0.000 min
Response: 299486097
Conc: 25.08 ng/ml

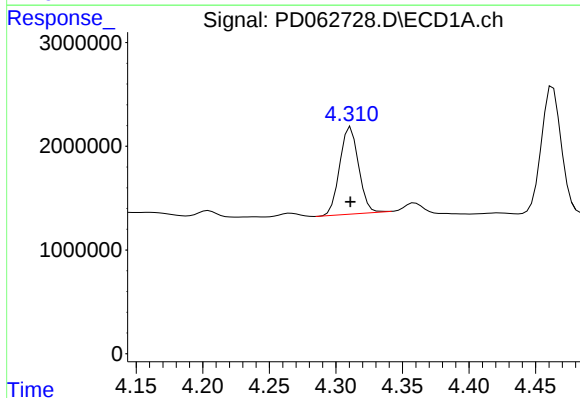


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 8267126
Conc: 232.65 ng/ml

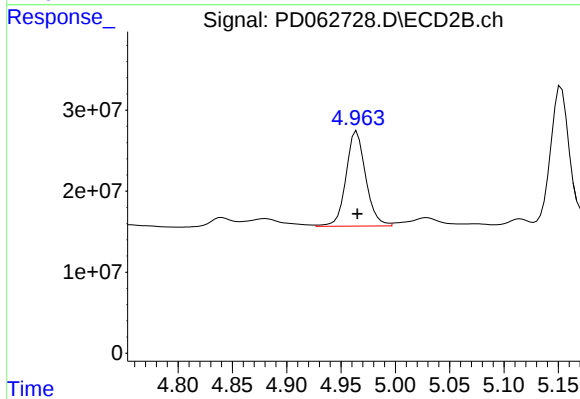

#23 Chlordane-1


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 148236211
Conc: 256.45 ng/ml

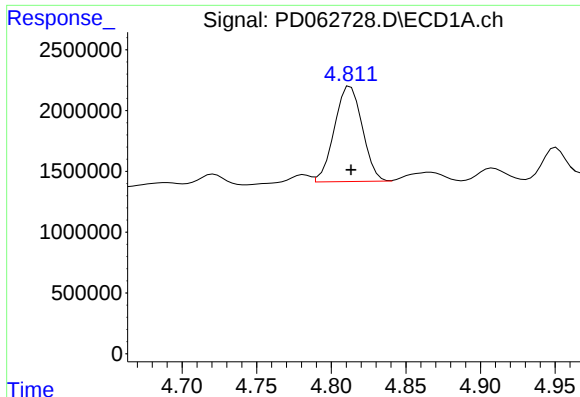

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 10205918
Conc: 250.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

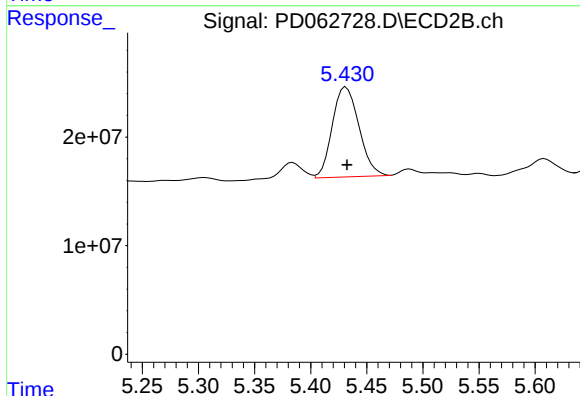


#24 Chlordane-2

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 136881240
Conc: 253.43 ng/ml

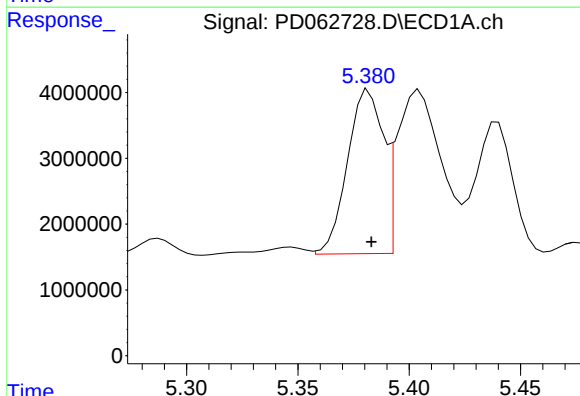


#25 Chlordane-3

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 27824811
Conc: 226.82 ng/ml

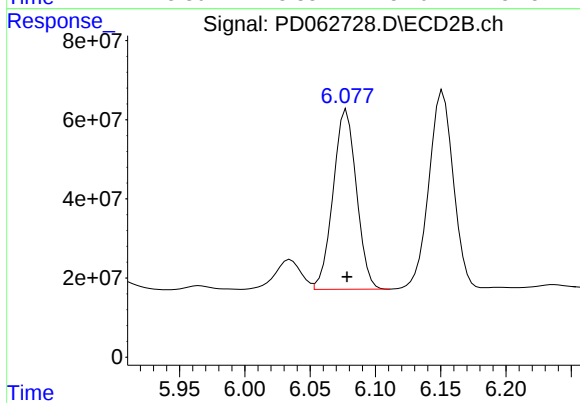

#25 Chlordane-3


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 565352852
Conc: 251.33 ng/ml

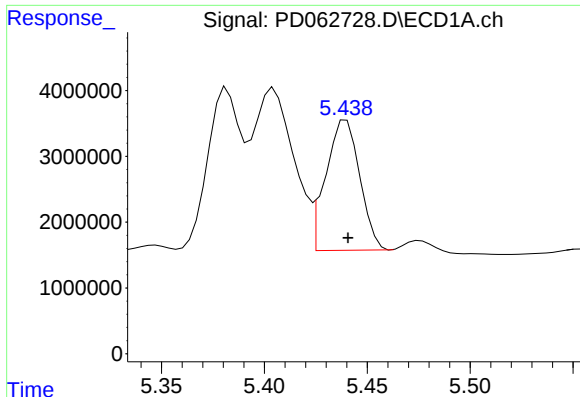

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 22736335
Conc: 224.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

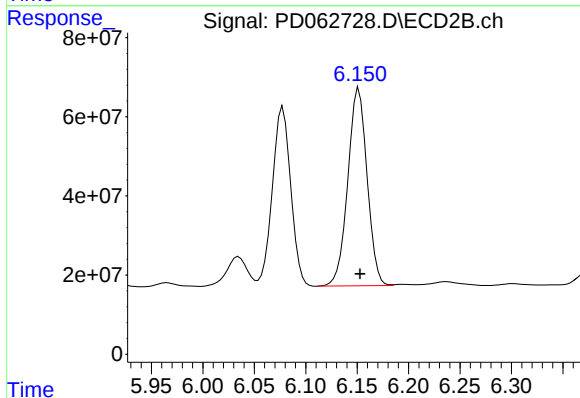


#26 Chlordane-4

R.T.: 6.152 min
Delta R.T.: -0.001 min
Response: 652240883
Conc: 252.89 ng/ml

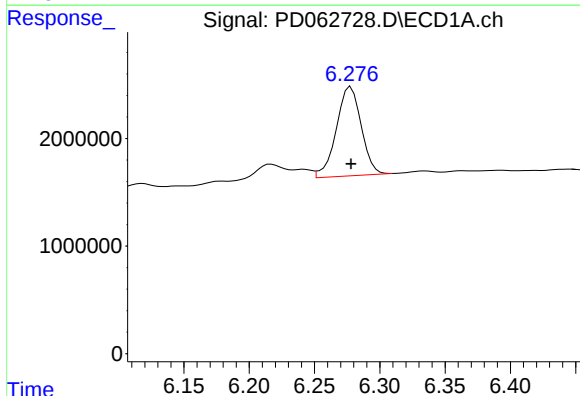


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 11002243
Conc: 247.70 ng/ml

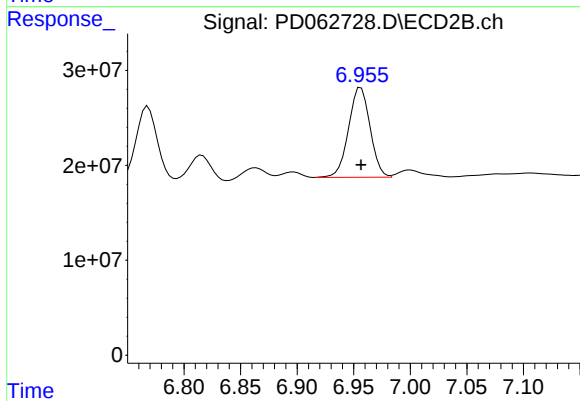

#27 Chlordane-5


R.T.: 6.956 min
Delta R.T.: 0.000 min
Response: 125156518
Conc: 253.86 ng/ml

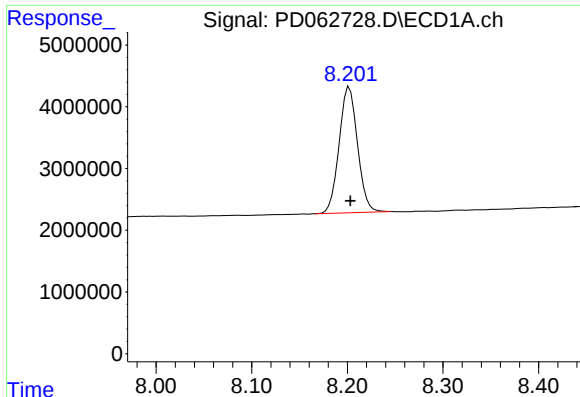

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 27354214
Conc: 24.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

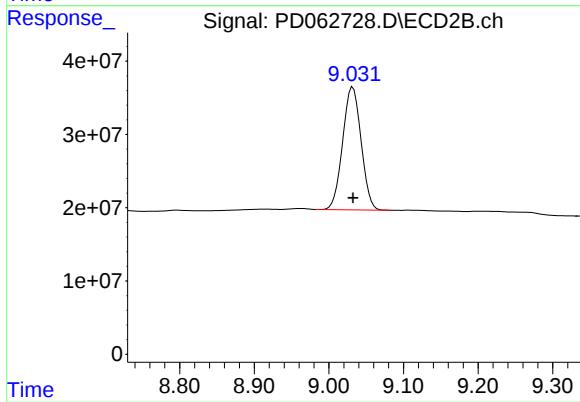

#28 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.000 min
Response: 287893765
Conc: 24.91 ng/ml