

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
 Data File : PD062741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2021 21:01
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 05:49:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 04:53:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	49969022	555.9E6	56.195	48.019
28)	SA Decachlor...	8.202	9.031	51994719	559.9E6	49.111	48.522
Target Compounds							
23)	Chlordane-1	4.311	4.964	16411386	271.7E6	465.396	473.844
24)	Chlordane-2	4.812	5.432	19022410	252.5E6	467.060	472.913
25)	Chlordane-3	5.382	6.078	56098350	1056.8E6	473.423	472.850
26)	Chlordane-4	5.440	6.152	46807883	1213.5E6	482.680	470.484
27)	Chlordane-5	6.277	6.956	20774875	234.2E6	476.567	476.084



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
Data File : PD062741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2021 21:01
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 05:49:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 04:53:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

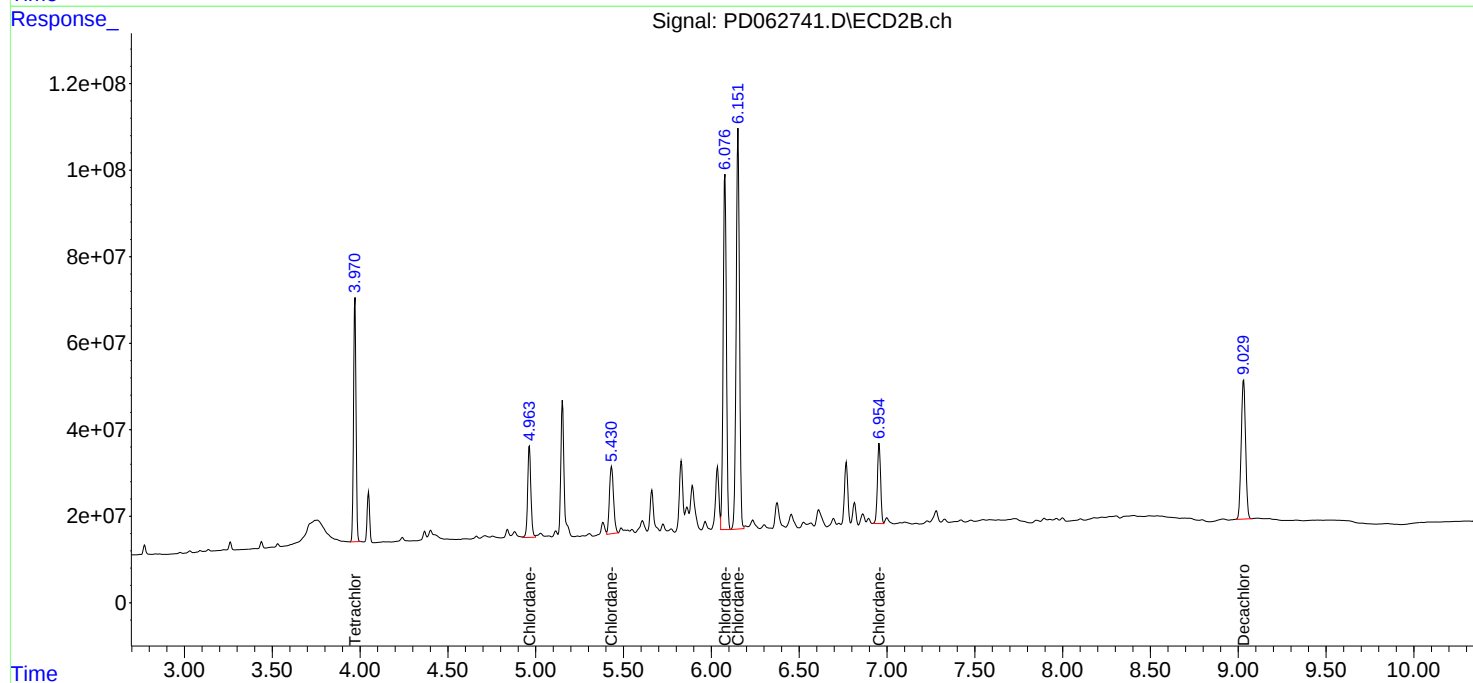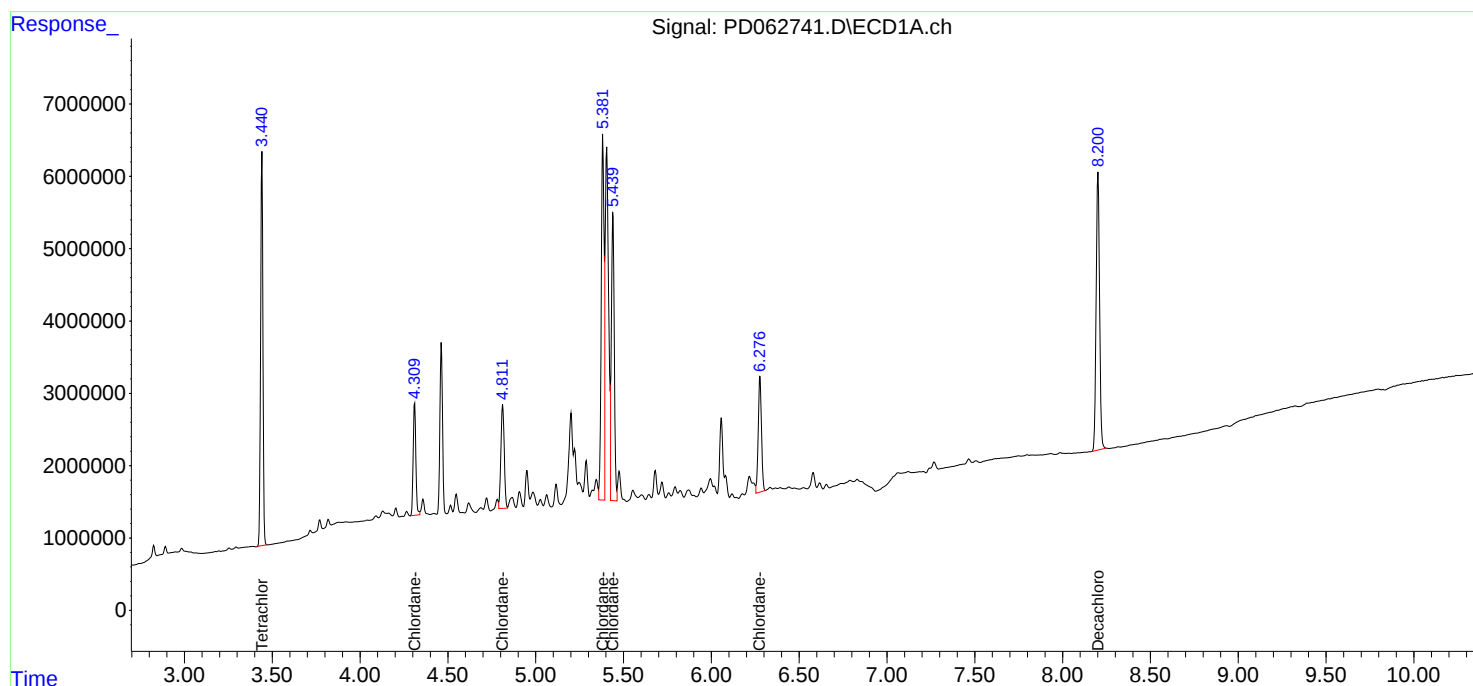


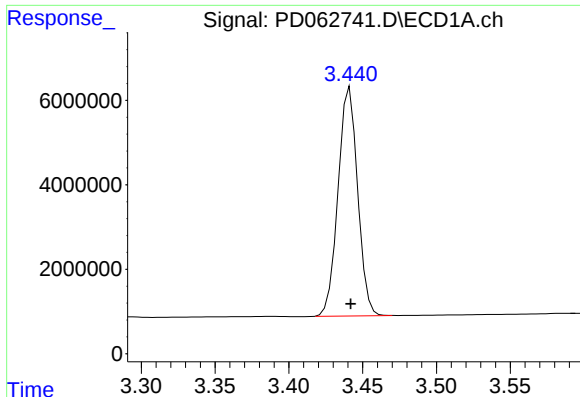

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 49969022
Conc: 56.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

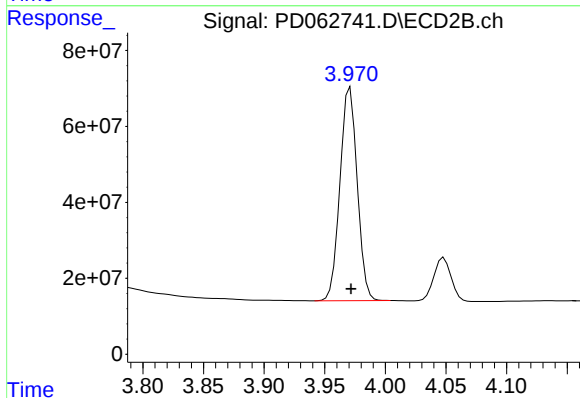


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 555916915
Conc: 48.02 ng/ml

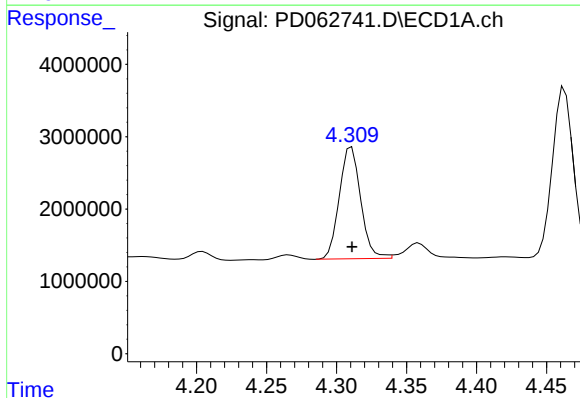


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 16411386
Conc: 465.40 ng/ml

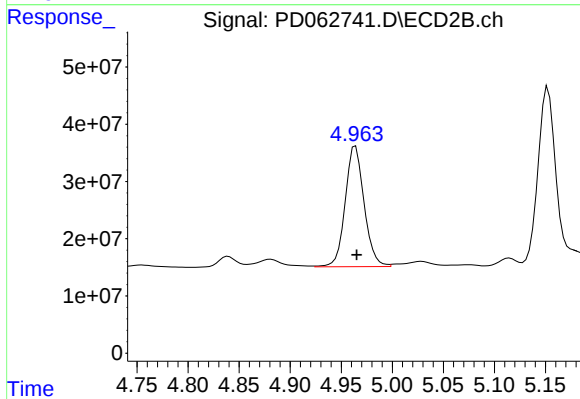

#23 Chlordane-1


R.T.: 4.964 min
Delta R.T.: -0.001 min
Response: 271713261
Conc: 473.84 ng/ml

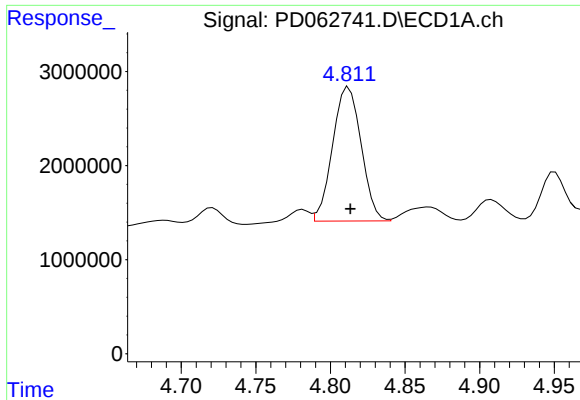

#24 Chlordane-2


R.T.: 4.812 min
Delta R.T.: 0.000 min
Response: 19022410
Conc: 467.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

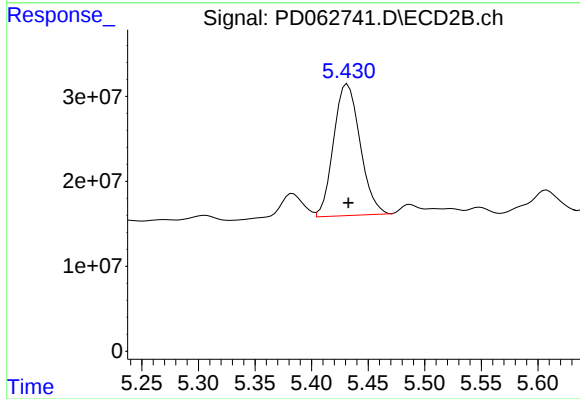


#24 Chlordane-2

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 252473662
Conc: 472.91 ng/ml

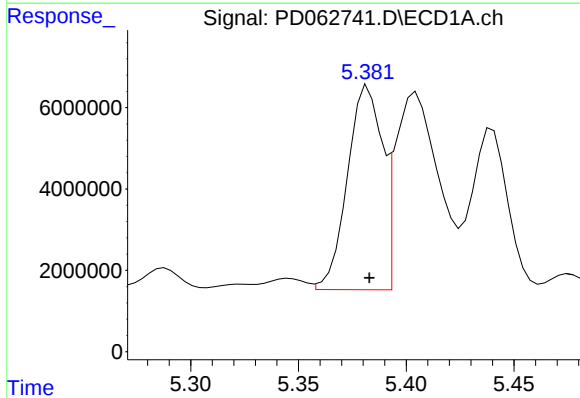


#25 Chlordane-3

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 56098350
Conc: 473.42 ng/ml

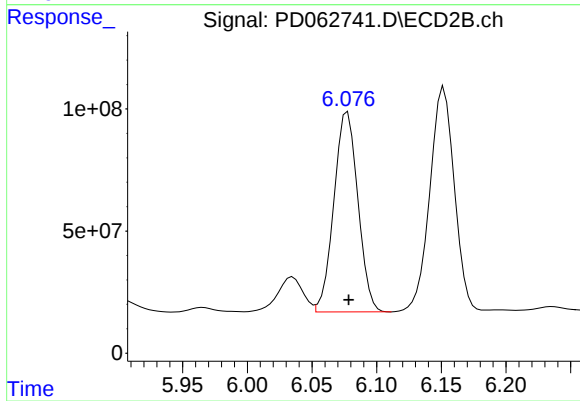

#25 Chlordane-3


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 1056779311
Conc: 472.85 ng/ml

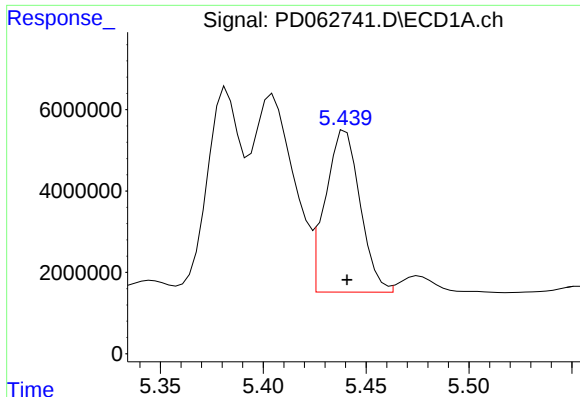

#26 Chlordane-4


R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 46807883
Conc: 482.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

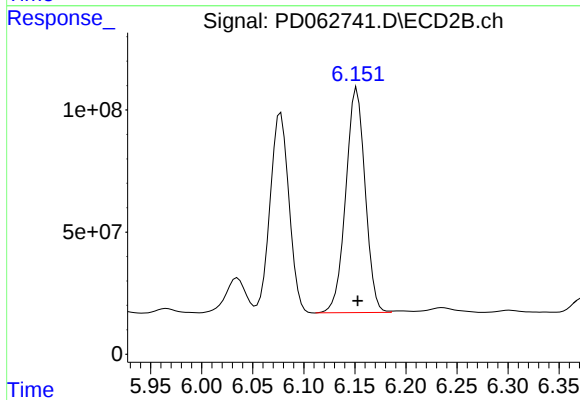


#26 Chlordane-4

R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 1213516375
Conc: 470.48 ng/ml

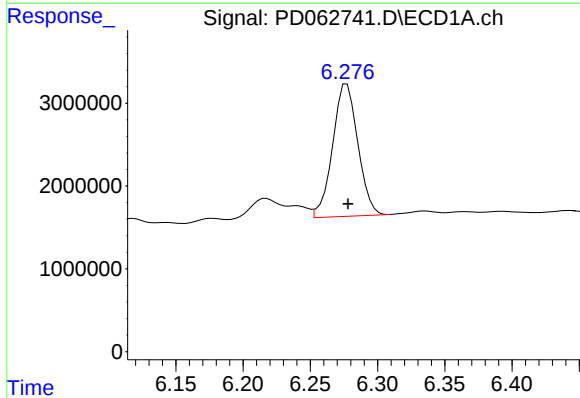


#27 Chlordane-5

R.T.: 6.277 min
Delta R.T.: 0.000 min
Response: 20774875
Conc: 476.57 ng/ml

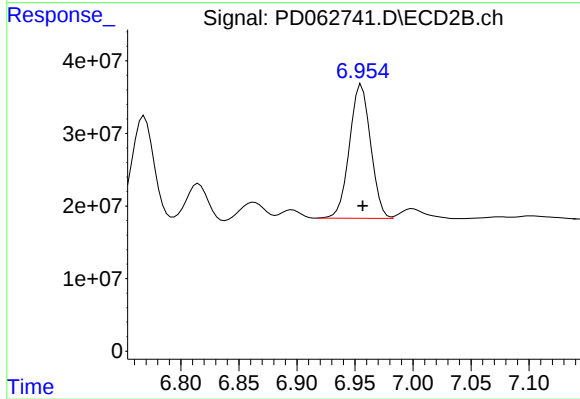

#27 Chlordane-5

R.T.: 6.956 min
Delta R.T.: 0.000 min
Response: 234159088
Conc: 476.08 ng/ml

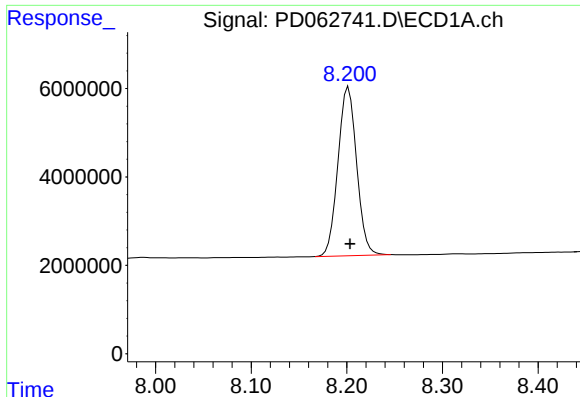

#28 Decachlorobiphenyl


R.T.: 8.202 min

Delta R.T.: -0.002 min

Response: 51994719

Conc: 49.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

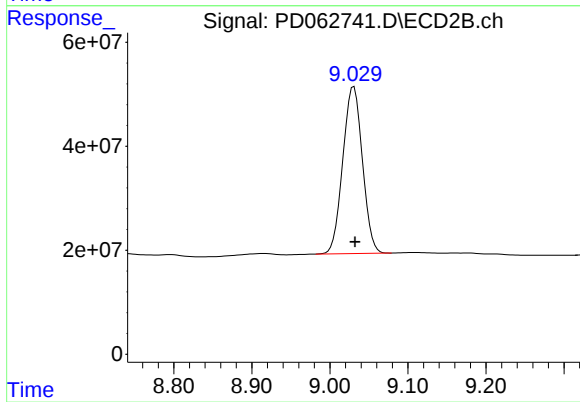

#28 Decachlorobiphenyl

R.T.: 9.031 min

Delta R.T.: -0.001 min

Response: 559898090

Conc: 48.52 ng/ml