

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
 Data File : PD062758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2021 00:58
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 05:50:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 04:53:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	51276416	561.7E6	57.665	48.519
28)	SA Decachlor...	8.202	9.031	51602363	557.8E6	48.741	48.339
Target Compounds							
23)	Chlordane-1	4.311	4.964	16784037	271.8E6	475.964	473.982
24)	Chlordane-2	4.813	5.432	19691705	254.7E6	483.493	477.029
25)	Chlordane-3	5.383	6.077	56701926	1048.6E6	478.516	469.204
26)	Chlordane-4	5.441	6.152	47466972	1202.9E6	489.477	466.371
27)	Chlordane-5	6.278	6.956	20964833	235.5E6	480.925	478.878



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050621\
Data File : PD062758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2021 00:58
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 05:50:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 04:53:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

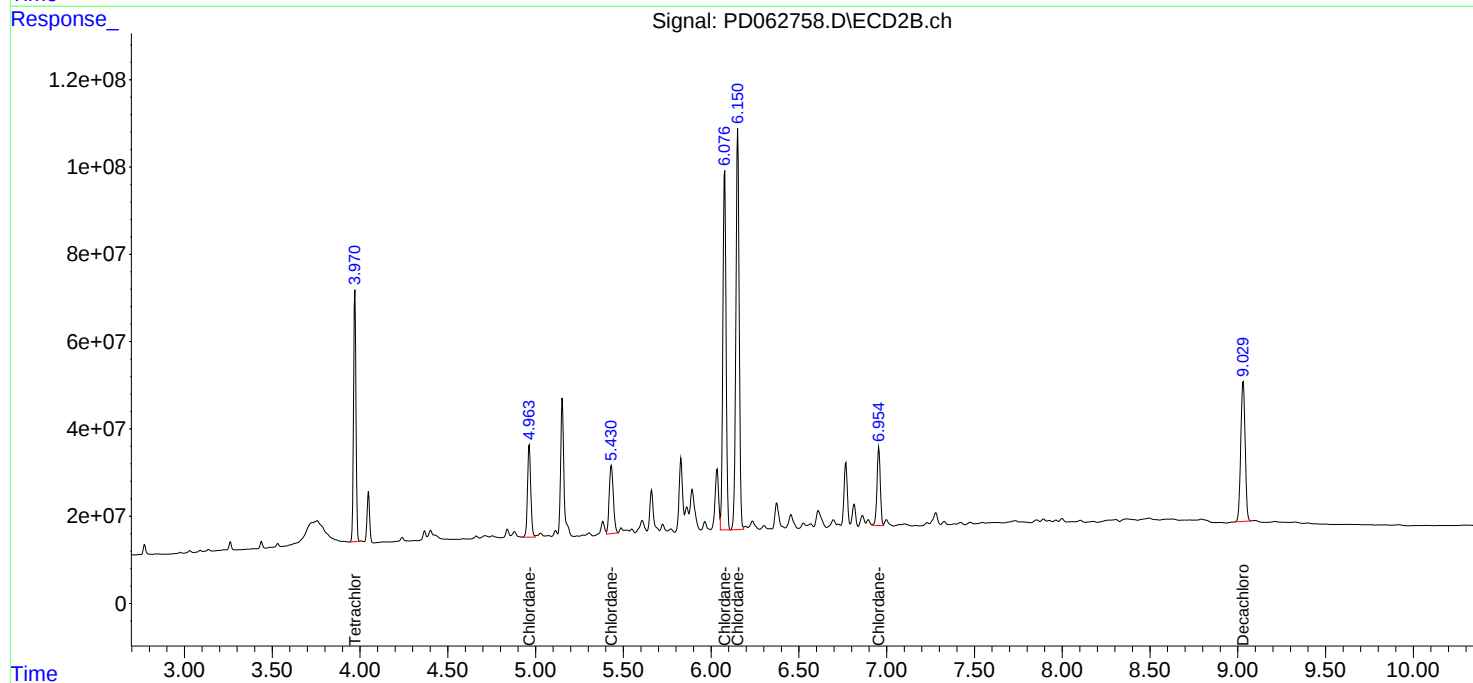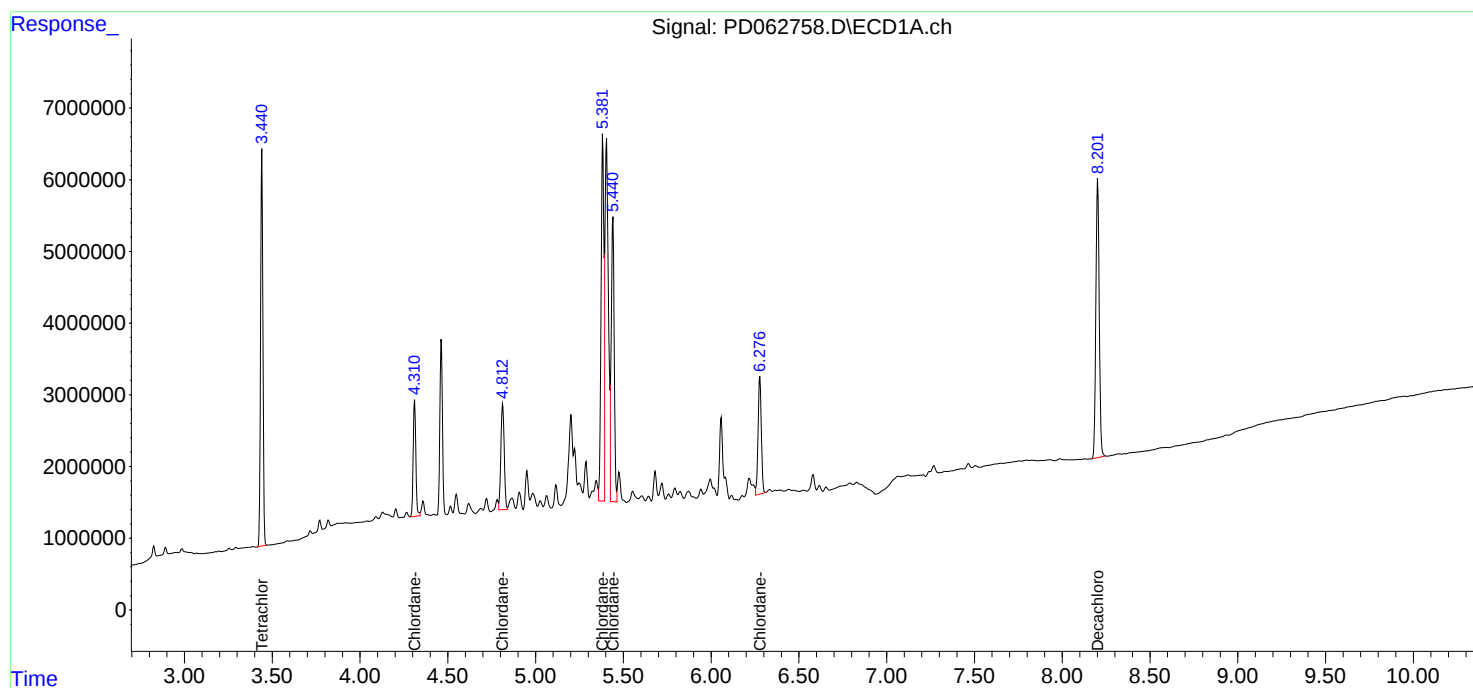


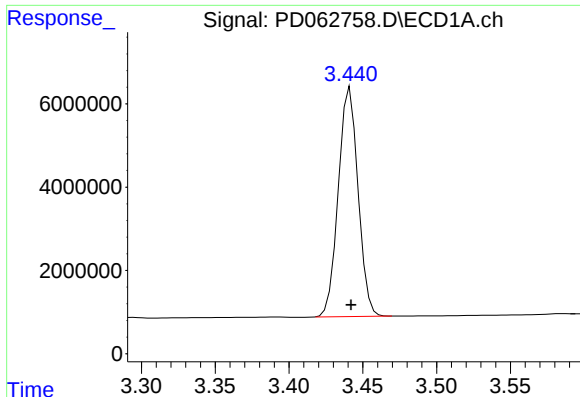

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 51276416
Conc: 57.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

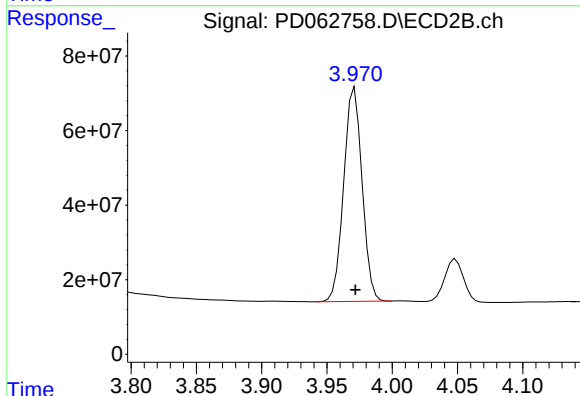


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 561706479
Conc: 48.52 ng/ml

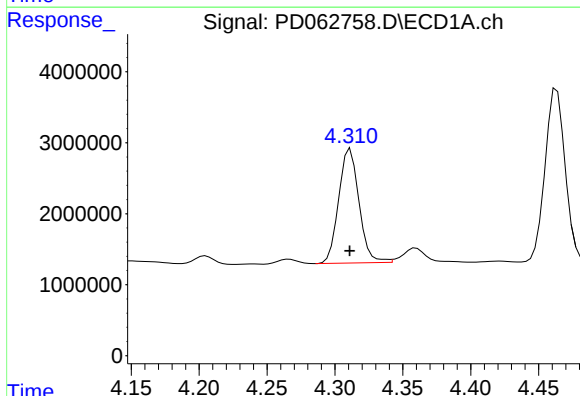


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 16784037
Conc: 475.96 ng/ml

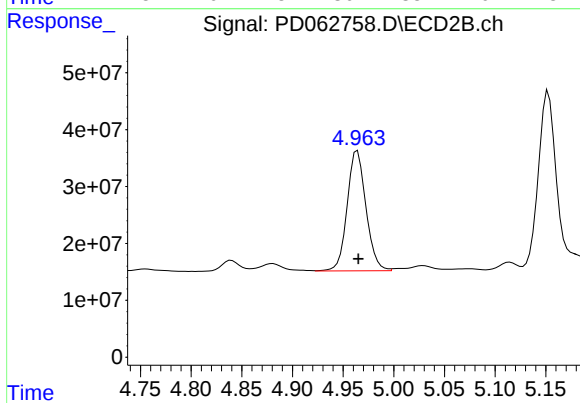

#23 Chlordane-1


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 271792713
Conc: 473.98 ng/ml

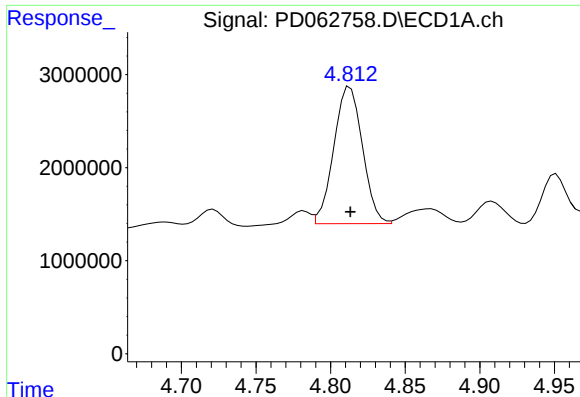

#24 Chlordane-2


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 19691705
Conc: 483.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

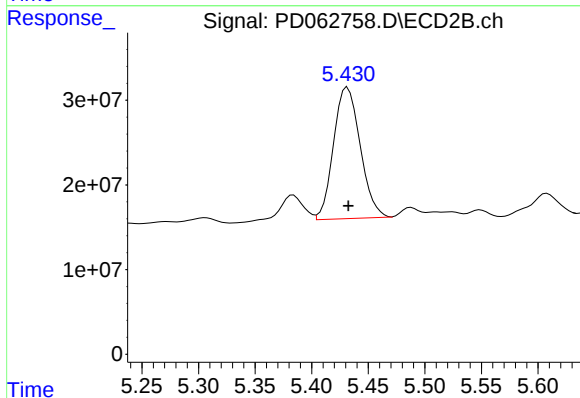


#24 Chlordane-2

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 254670959
Conc: 477.03 ng/ml

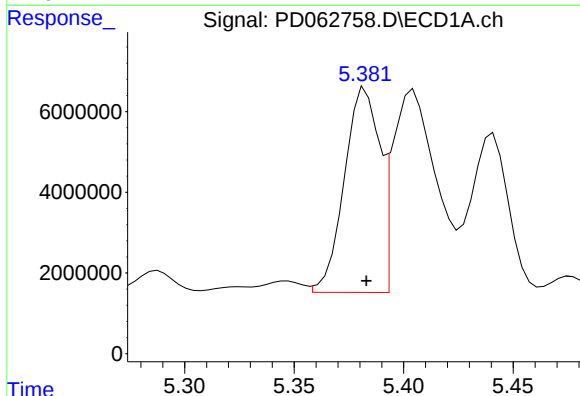


#25 Chlordane-3

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 56701926
Conc: 478.52 ng/ml

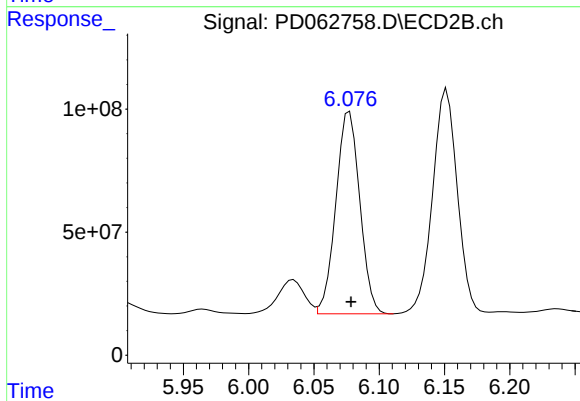

#25 Chlordane-3


R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 1048630322
Conc: 469.20 ng/ml

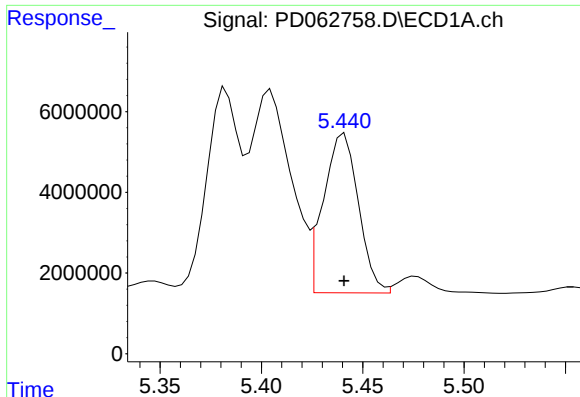

#26 Chlordane-4


R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 47466972
Conc: 489.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

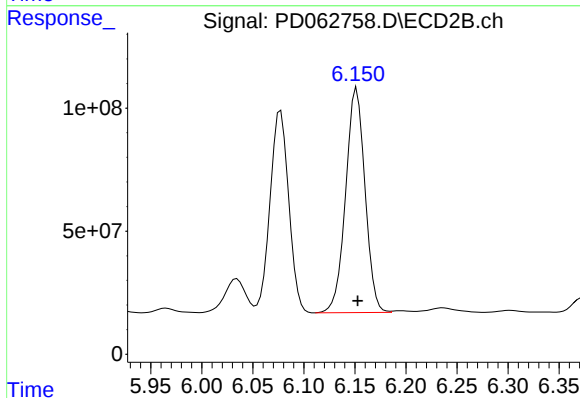


#26 Chlordane-4

R.T.: 6.152 min
Delta R.T.: -0.001 min
Response: 1202909256
Conc: 466.37 ng/ml

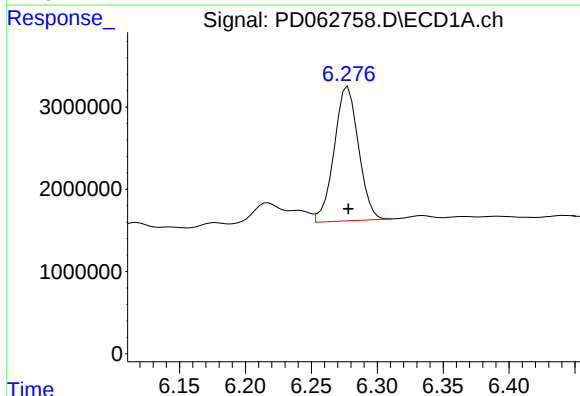


#27 Chlordane-5

R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 20964833
Conc: 480.92 ng/ml

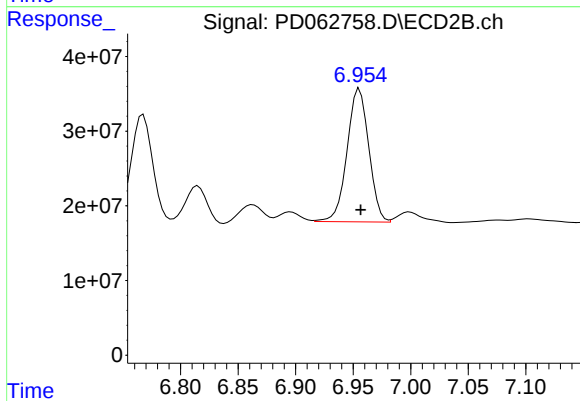

#27 Chlordane-5

R.T.: 6.956 min
Delta R.T.: -0.001 min
Response: 235533031
Conc: 478.88 ng/ml

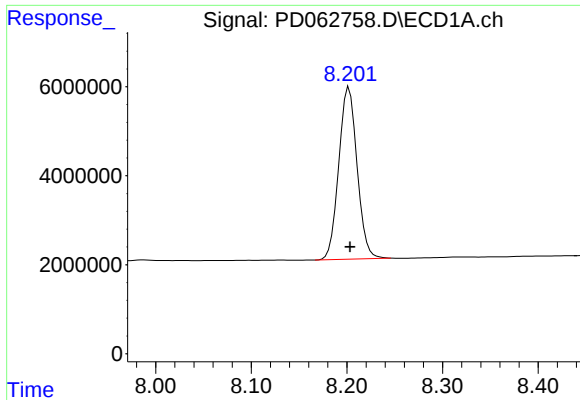

#28 Decachlorobiphenyl


R.T.: 8.202 min

Delta R.T.: -0.001 min

Response: 51602363

Conc: 48.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

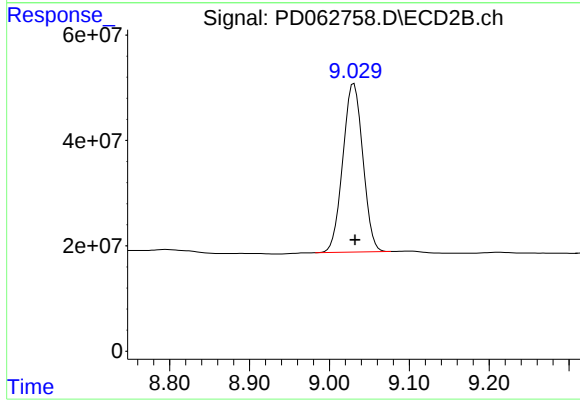

#28 Decachlorobiphenyl

R.T.: 9.031 min

Delta R.T.: -0.001 min

Response: 557782848

Conc: 48.34 ng/ml