

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050622\
 Data File : PD069449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2022 11:44
 Operator : AR\AJ
 Sample : N2697-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGBP8MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/09/2022
 Supervised By : mohammad ahmed 05/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 00:38:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	16924692	203.3E6	13.358	16.843 #
27)	SA Decachlor...	8.199	9.366	26460141	148.0E6	19.898	21.044
Target Compounds							
2)	A alpha-BHC	3.883	4.567	76329532	677.2E6	42.702	41.196m
3)	MA gamma-BHC...	4.167	4.859	75803874	649.9E6	41.908	41.716
4)	MA Heptachlor	4.464	5.385	76080211	644.0E6	44.810	42.541
5)	MB Aldrin	4.711	5.698	74602310	629.3E6	46.832	44.083
6)	B beta-BHC	4.417	5.021	34339805	243.7E6	44.334	36.324
7)	B delta-BHC	4.620	5.248	22911723	159.4E6	14.354	13.575
8)	B Heptachlo...	5.155	6.087	67860734	526.1E6	46.099	47.224
9)	A Endosulfan I	5.495	6.448	59704124	512.7E6	40.914	43.163
10)	B trans-Chl...	5.381	6.323	70611119	563.4E6	47.100	44.411
11)	B cis-Chlor...	5.440	6.398	67892670	541.6E6	45.485	43.489
12)	B 4,4'-DDE	5.605	6.547	135.0E6	985.3E6	100.654	90.568
13)	MA Dieldrin	5.737	6.707	147.6E6	1040.8E6	94.847	86.291
14)	MA Endrin	5.995	6.927	122.2E6	843.2E6	87.308	86.703
15)	B Endosulfa...	6.269	7.132	114.8E6	817.2E6	89.084	85.263
16)	A 4,4'-DDD	6.123	7.038	106.3E6	799.0E6	87.183	85.322
17)	MA 4,4'-DDT	6.362	7.341	105.7E6	769.5E6	86.147	85.476
18)	B Endrin al...	6.439	7.256	91190681	651.9E6	91.868	91.244
19)	B Endosulfa...	6.651	7.482	90655650	689.5E6	72.351	78.585
20)	A Methoxychlor	6.913	7.794	278.4E6	1698.2E6	410.196	412.071
21)	B Endrin ke...	7.144	7.956	127.4E6	791.3E6	88.164	85.713

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050622\
Data File : PD069449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2022 11:44
Operator : AR\AJ
Sample : N2697-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 00:38:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

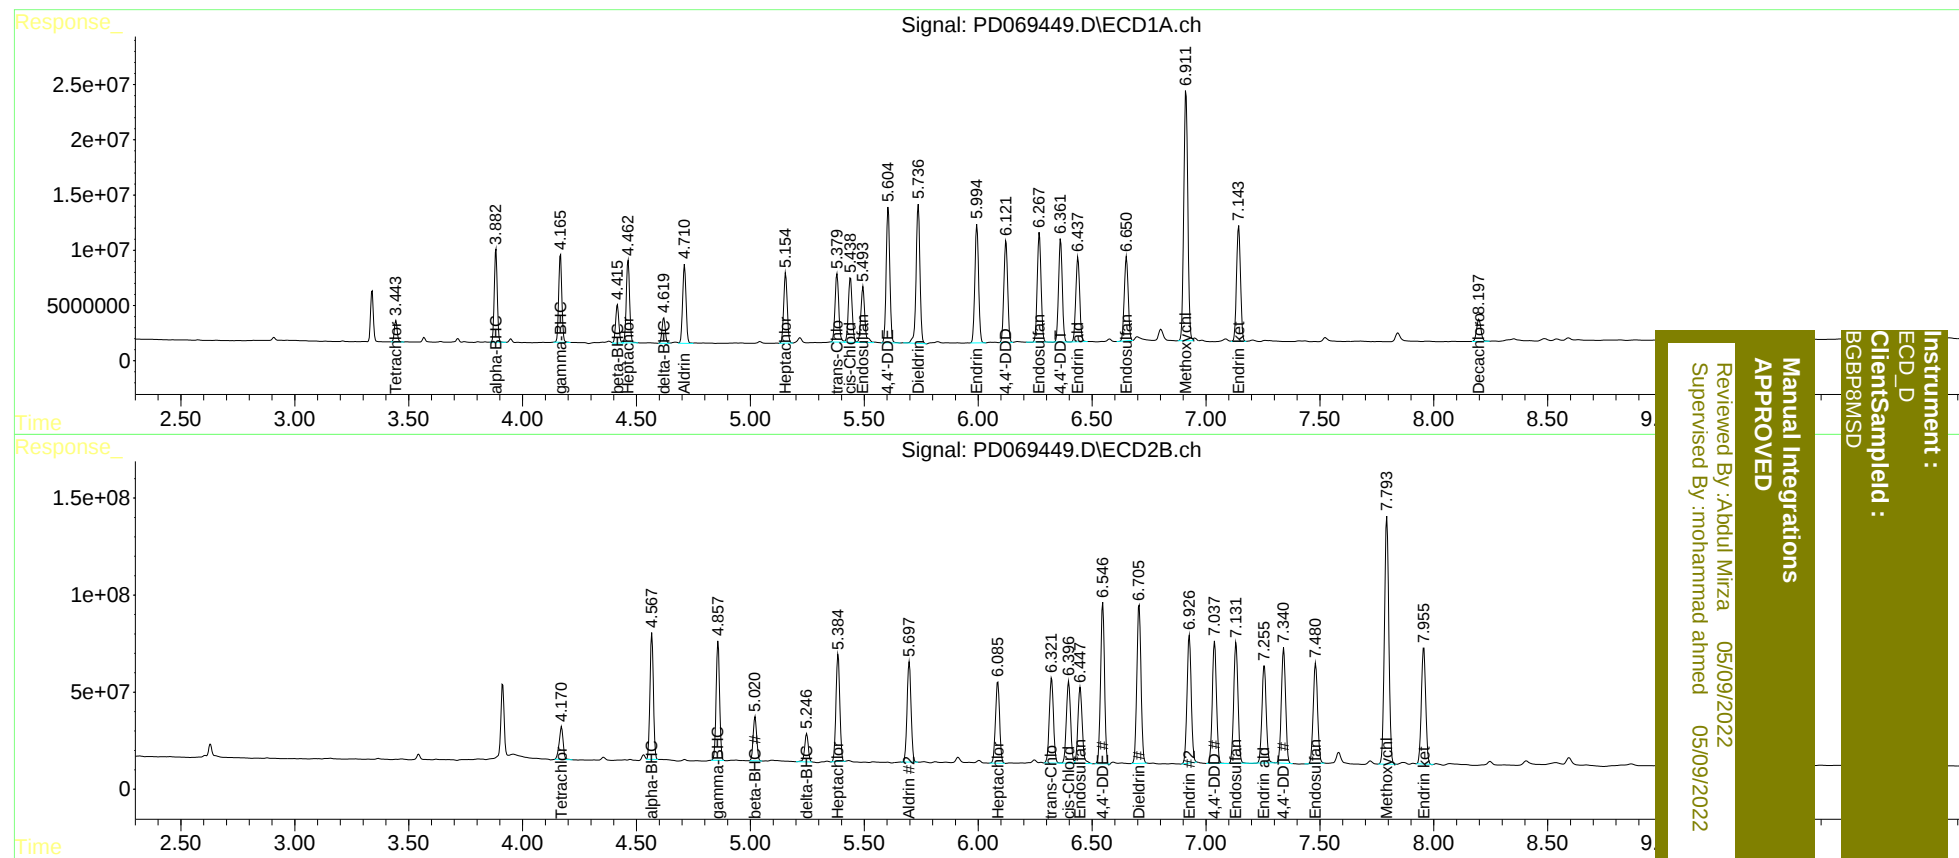

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 05/09/2022
Supervised By: mohammad ahmed 05/09/2022

Instrument :
ECD_D
ClientSampled :
BGBP8MSD