

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050622\
 Data File : PD069448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2022 11:30
 Operator : AR\AJ
 Sample : N2697-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGBP8MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/09/2022
 Supervised By : mohammad ahmed 05/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 00:38:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	16777117	206.6E6	13.242	17.115 #
27)	SA Decachlor...	8.200	9.365	27028615	152.2E6	20.326	21.643
Target Compounds							
2)	A alpha-BHC	3.884	4.566	75264222	687.8E6	42.106	41.839m
3)	MA gamma-BHC...	4.167	4.858	74577583	655.8E6	41.230	42.093
4)	MA Heptachlor	4.464	5.385	74586708	652.2E6	43.930	43.082
5)	MB Aldrin	4.711	5.698	73843514	636.7E6	46.355	44.601
6)	B beta-BHC	4.417	5.021	33938199	247.7E6	43.815	36.919
7)	B delta-BHC	4.621	5.247	22736095	160.2E6	14.244	13.644
8)	B Heptachlo...	5.155	6.086	67528965	529.1E6	45.874	47.490
9)	A Endosulfan I	5.495	6.449	62123620	523.2E6	42.572	44.048
10)	B trans-Chl...	5.381	6.323	70476789	570.8E6	47.010	44.994
11)	B cis-Chlor...	5.440	6.398	68989009	553.0E6	46.219	44.402
12)	B 4,4'-DDE	5.606	6.547	135.1E6	1005.0E6	100.700	92.382
13)	MA Dieldrin	5.738	6.707	146.5E6	1061.9E6	94.105	88.040
14)	MA Endrin	5.996	6.928	121.1E6	850.2E6	86.580	87.426
15)	B Endosulfa...	6.269	7.133	114.3E6	831.5E6	88.726	86.757
16)	A 4,4'-DDD	6.123	7.039	106.6E6	811.5E6	87.403	86.665
17)	MA 4,4'-DDT	6.363	7.342	105.1E6	782.4E6	85.670	86.919
18)	B Endrin al...	6.440	7.256	91297927	663.7E6	91.976	92.891
19)	B Endosulfa...	6.651	7.482	90997135	699.1E6	72.623	79.672
20)	A Methoxychlor	6.914	7.795	275.9E6	1716.3E6	406.490	416.481
21)	B Endrin ke...	7.145	7.956	127.7E6	816.2E6	88.383	88.408

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050622\
Data File : PD069448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2022 11:30
Operator : AR\AJ
Sample : N2697-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 00:38:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

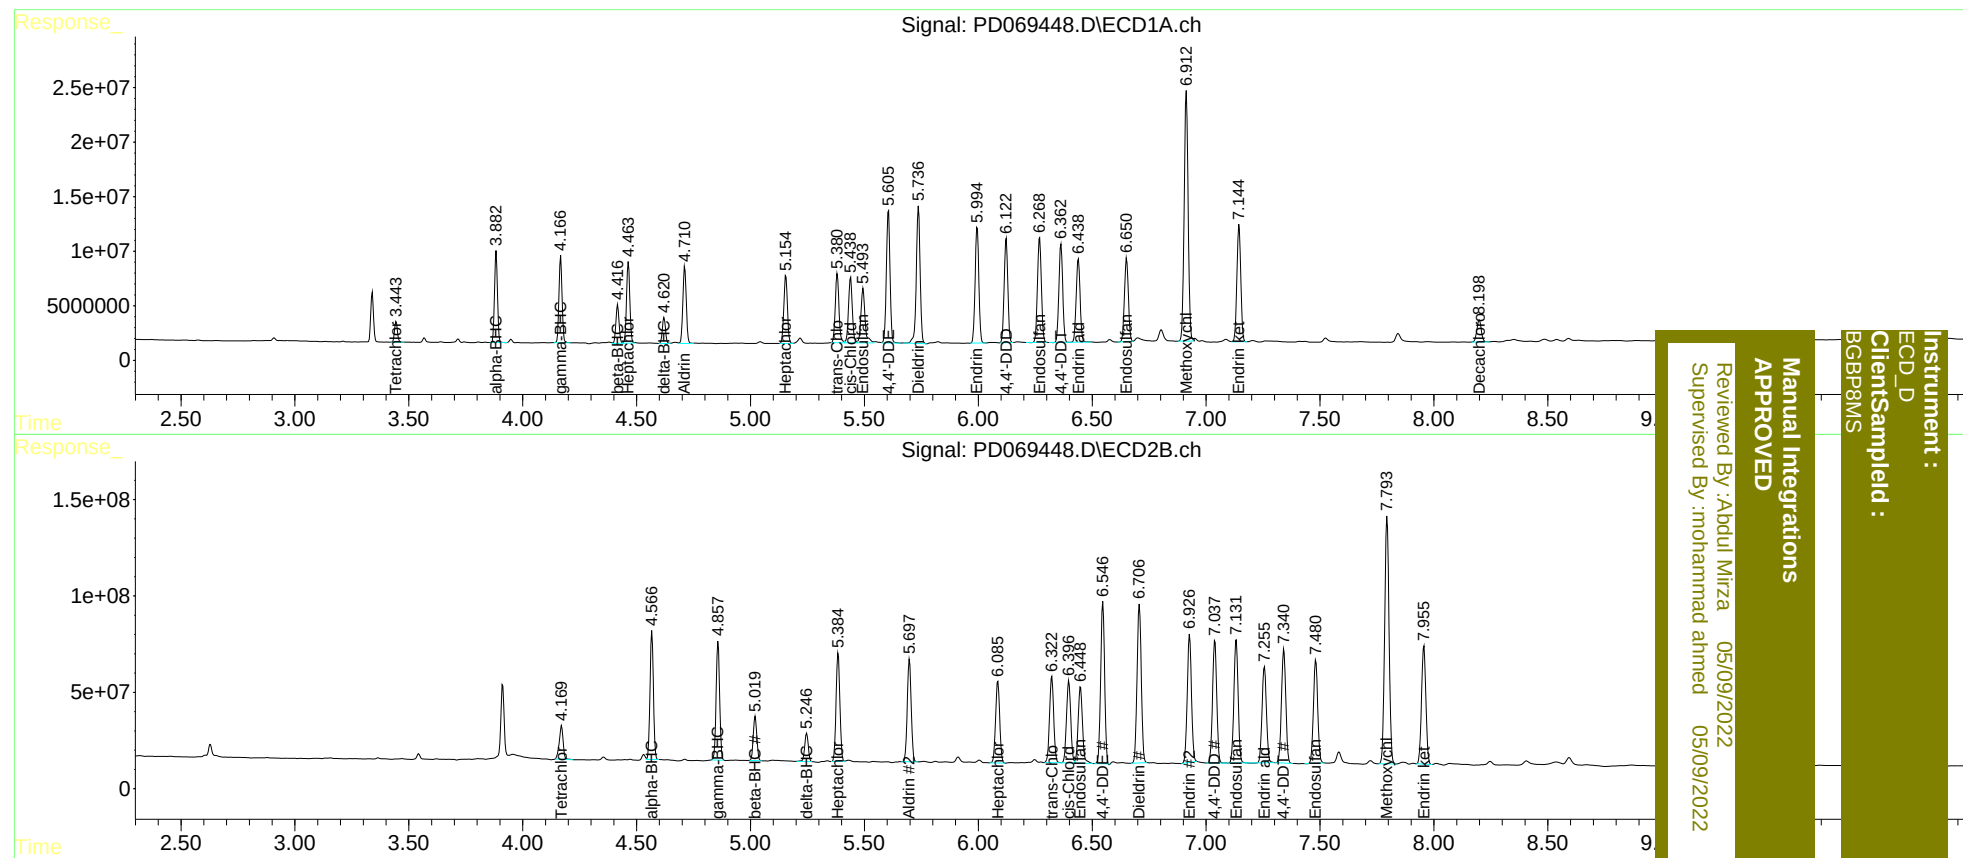

Reviewed By: Abdul Mirza 05/09/2022
Supervised By: mohammad ahmed 05/09/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGBP8MS