

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050623\
 Data File : PD075320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2023 11:41
 Operator : AR\AJ
 Sample : 02479-12DL2 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW953DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/09/2023
 Supervised By : Ankita Jodhani 05/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 07:24:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
3) MA	gamma-BHC...	4.342	3.613	24366507	1645616	6.778m 1.120 #
15) B	Endosulfa...	6.837	5.918	1480.0E6	75316563	459.558m 58.865m#
17) MA	4,4'-DDT	7.013	6.032	212.8E6	104.9E6	83.824m 104.130
19) B	Endosulfa...	7.155	6.331	14100522	10728835	5.126m 9.225m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050623\
Data File : PD075320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2023 11:41
Operator : AR\AJ
Sample : 02479-12DL2 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 07:24:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

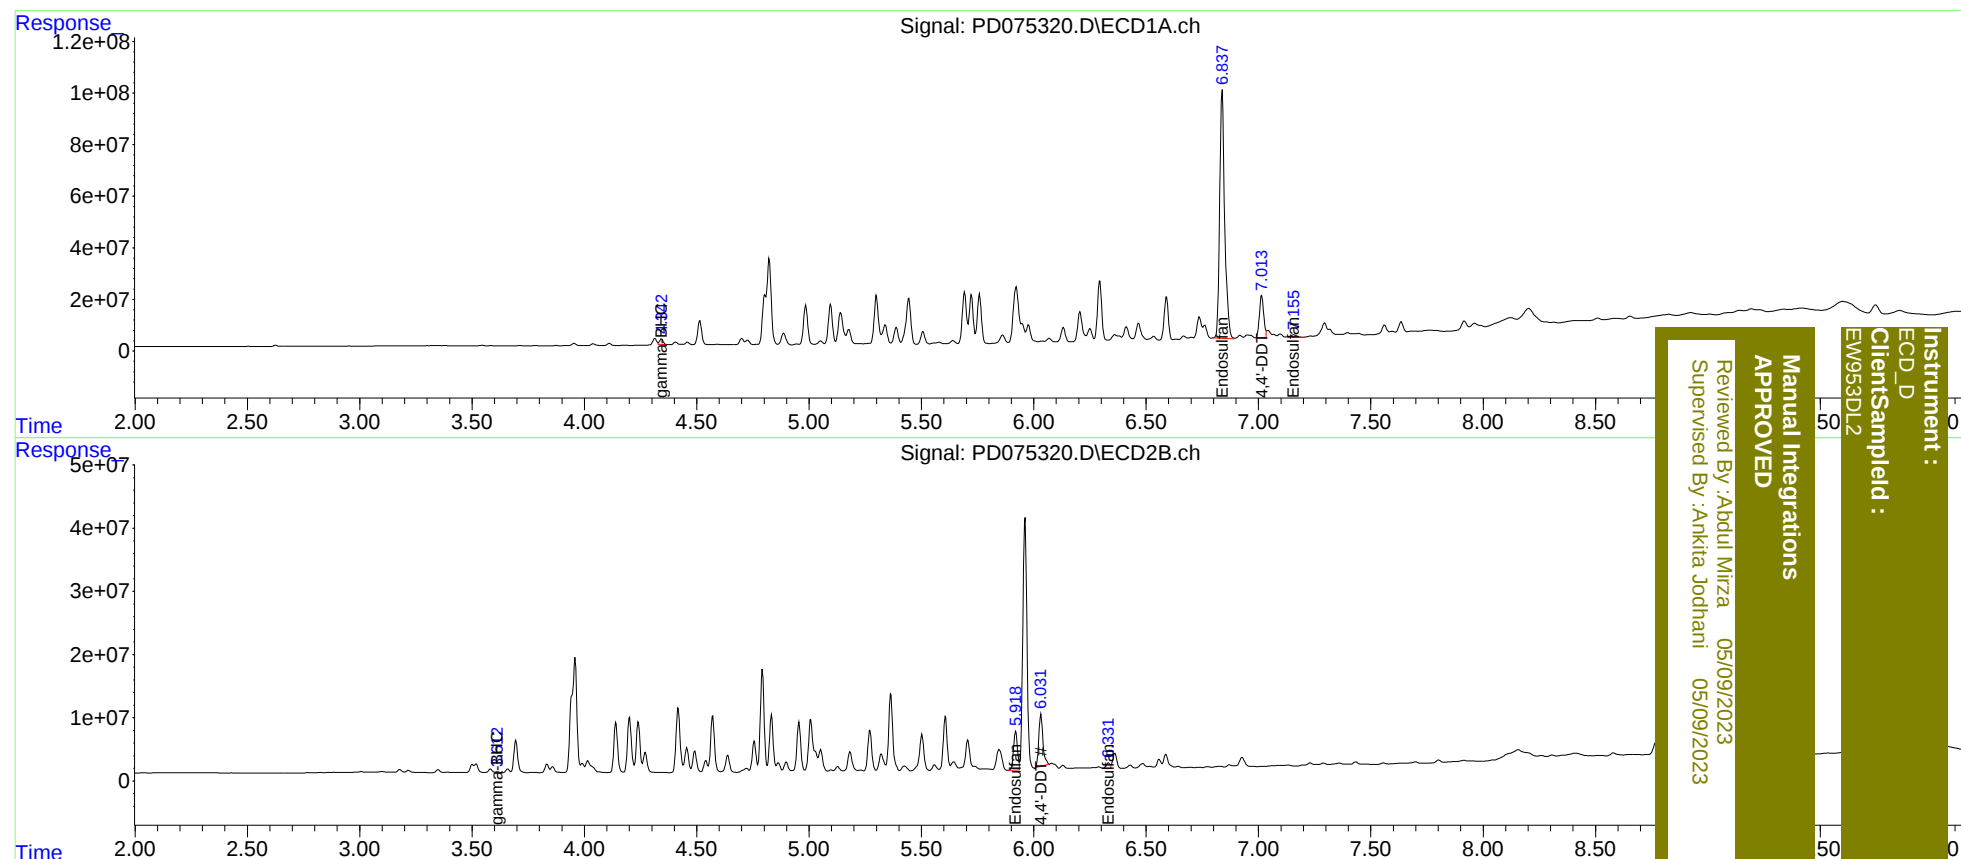

Reviewed By: Abdul Mirza 05/09/2023
Supervised By: Ankita Jodhani 05/09/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW/953DL2