

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050721\
 Data File : PD062760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2021 13:17
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 08:06:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.839	0	36848909	N.D. 2.307 #
9) A	Endosulfan I	0.000	6.185f	0	5995173	N.D. 0.406 #
15) B	Endosulfa...	0.000	6.896	0	21801838	N.D. 1.632 #
17) MA	4,4'-DDT	0.000	7.096	0	21777693	N.D. 1.710 #
19) B	Endosulfa...	0.000	7.213f	0	5614624	N.D. 0.404 #
22)	Mirex	0.000	8.157	0	45259898	N.D. 4.941 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050721\
Data File : PD062760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2021 13:17
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 08:06:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

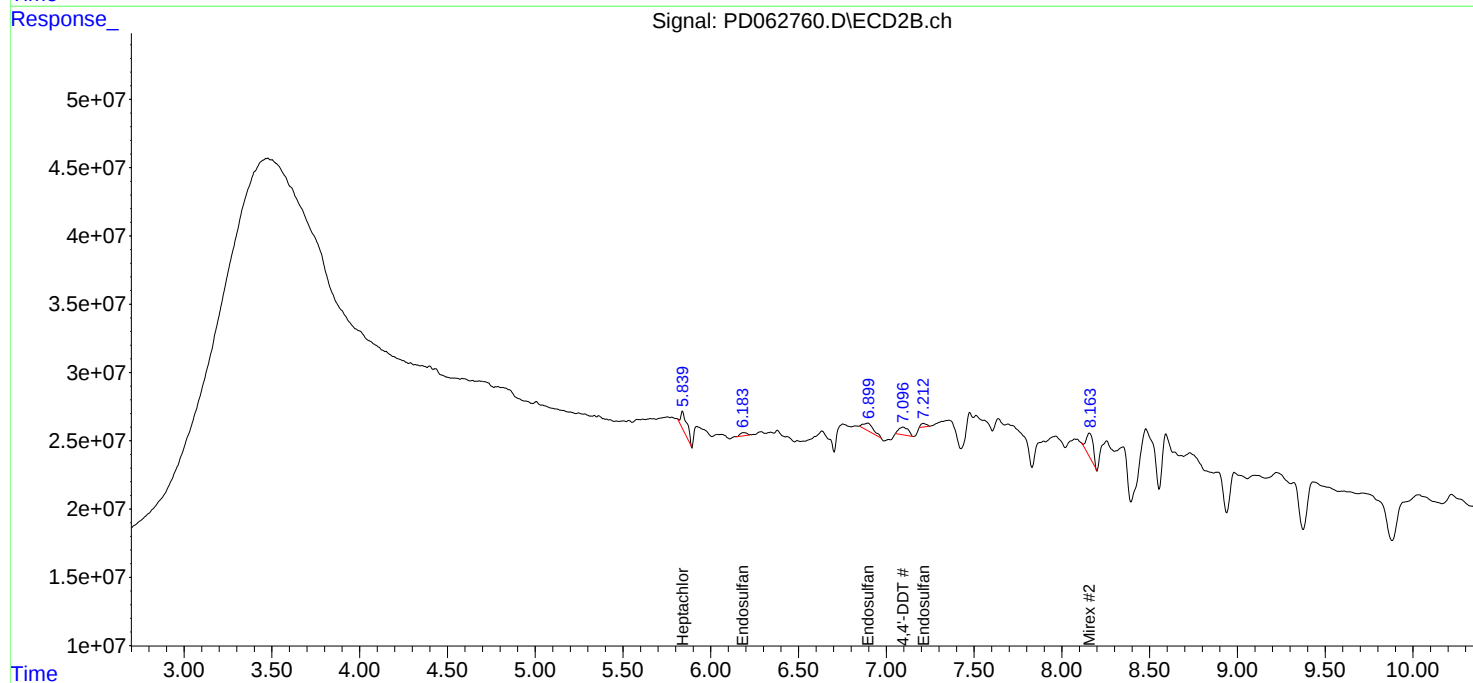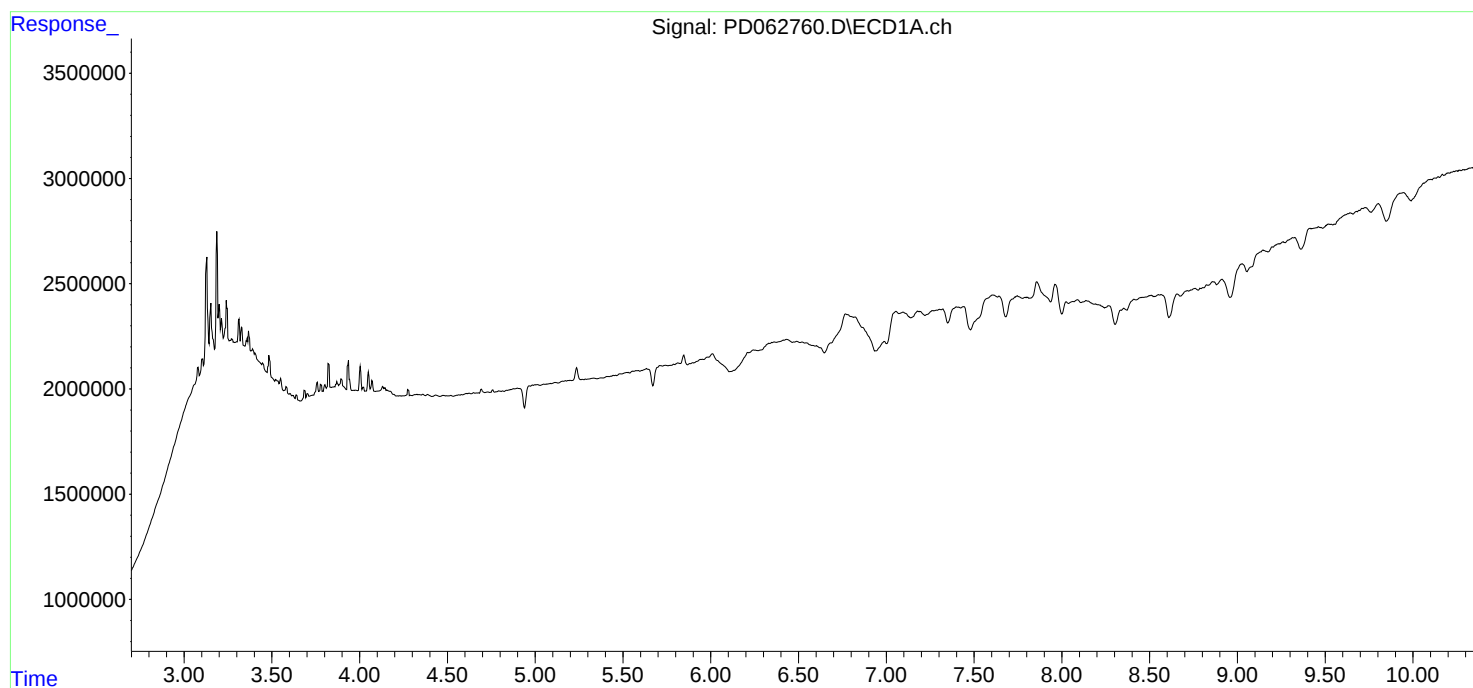


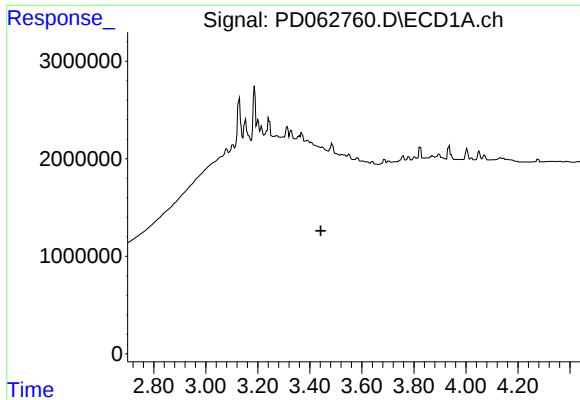

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

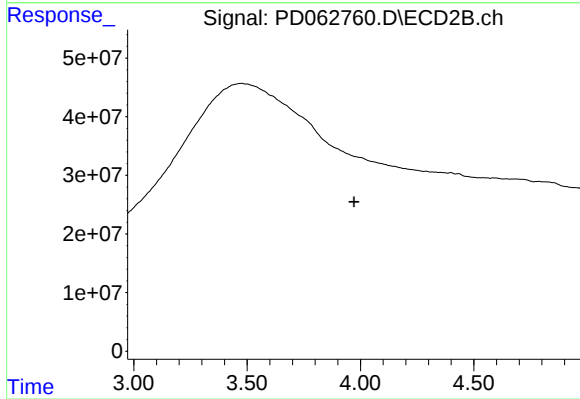


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.972 min
Response: 0
Conc: N.D.

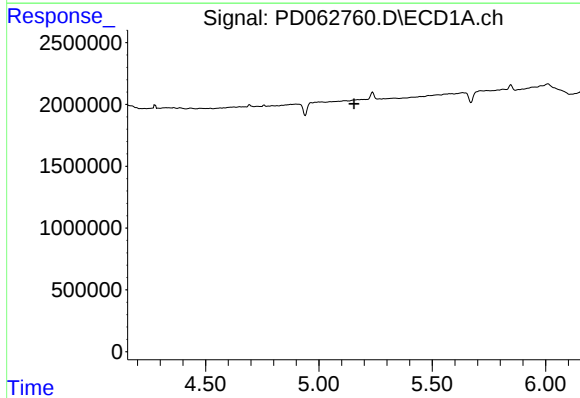


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

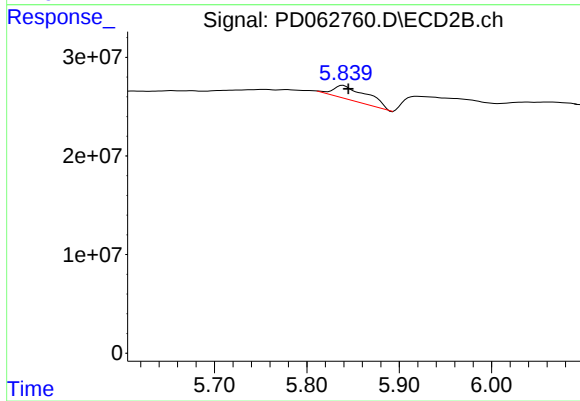

#8 Heptachlor epoxide


R.T.: 5.839 min
Delta R.T.: -0.006 min
Response: 36848909
Conc: 2.31 ng/ml

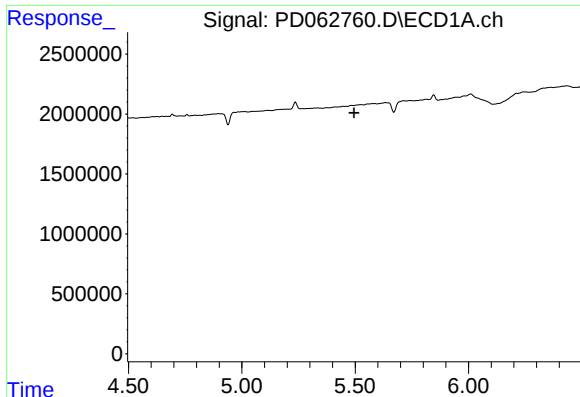

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

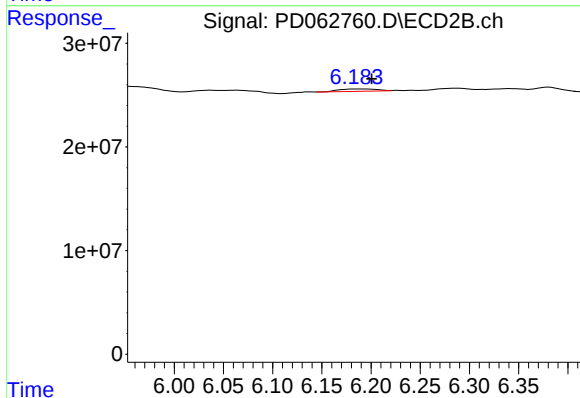


#9 Endosulfan I

R.T.: 6.185 min
Delta R.T.: -0.016 min
Response: 5995173
Conc: 0.41 ng/ml

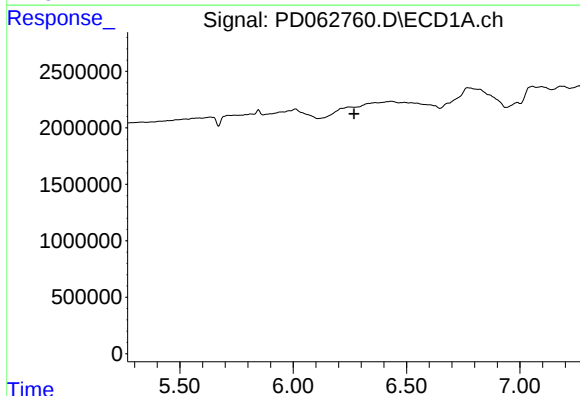


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.269 min
Response: 0
Conc: N.D.

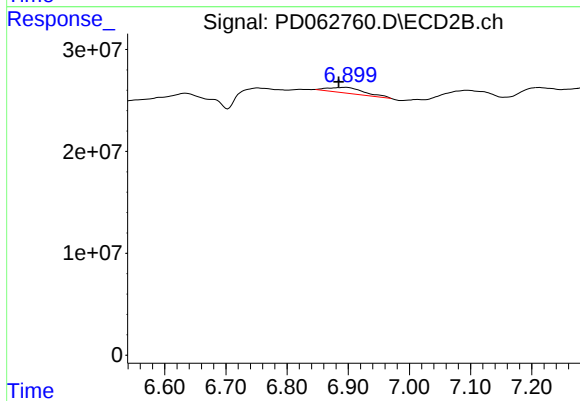

#15 Endosulfan II


R.T.: 6.896 min
Delta R.T.: 0.012 min
Response: 21801838
Conc: 1.63 ng/ml

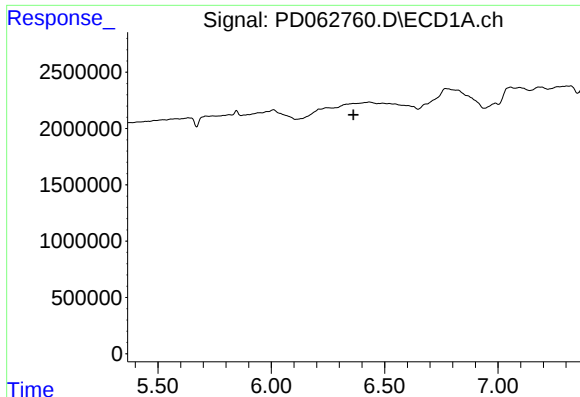

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

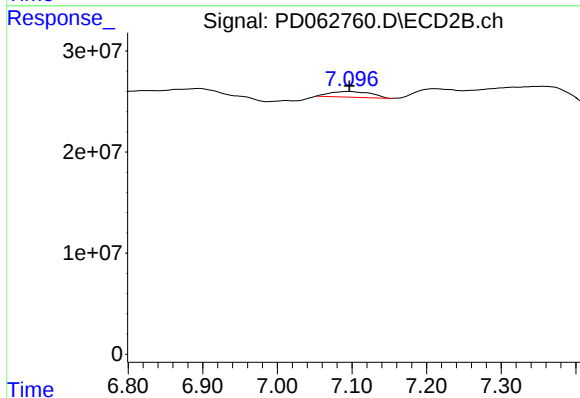


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: 0.000 min
Response: 21777693
Conc: 1.71 ng/ml

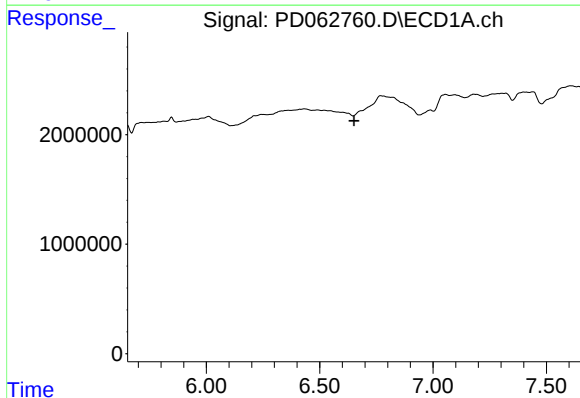


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.651 min
Response: 0
Conc: N.D.

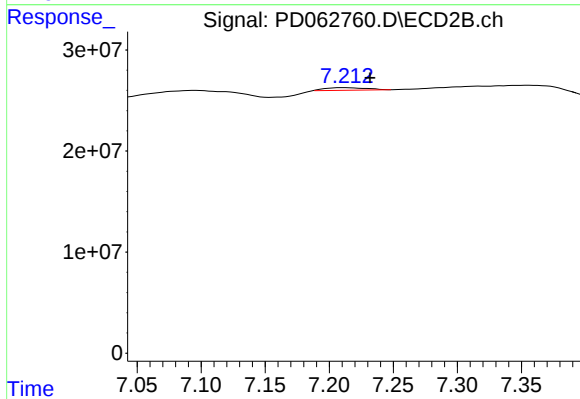

#19 Endosulfan Sulfate


R.T.: 7.213 min
Delta R.T.: -0.019 min
Response: 5614624
Conc: 0.40 ng/ml

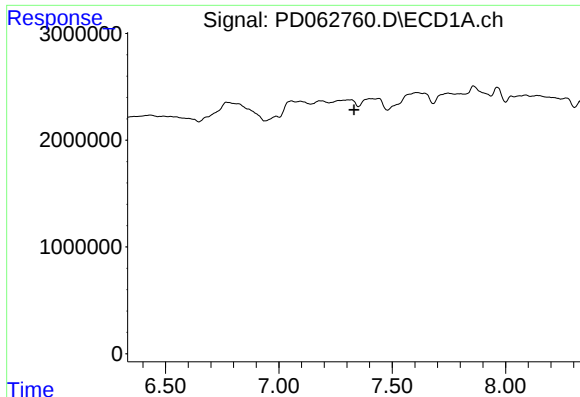

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

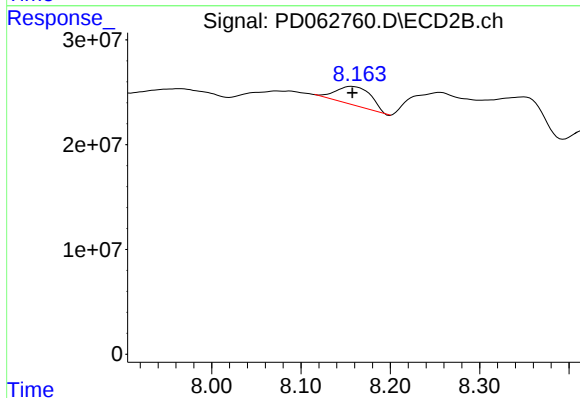


#22 Mirex

R.T.: 8.157 min
Delta R.T.: 0.000 min
Response: 45259898
Conc: 4.94 ng/ml

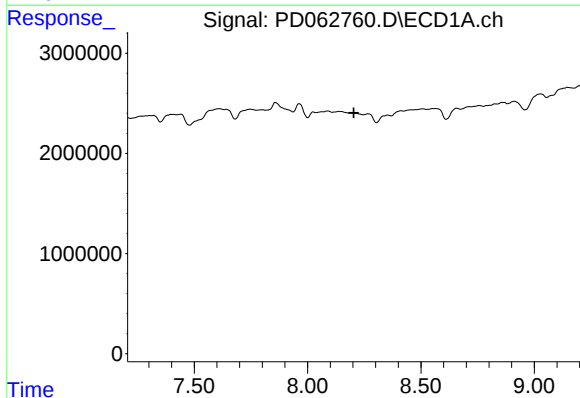

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.203 min
Response: 0
Conc: N.D.

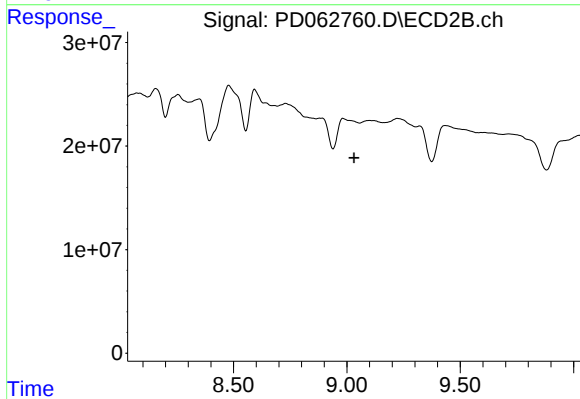

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.032 min
Response: 0
Conc: N.D.