

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050721\
 Data File : PD062787.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2021 19:49
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 09:33:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	50123758	545.7E6	56.369	47.134
28)	SA Decachlor...	8.201	9.030	51760069	555.4E6	48.890	48.137
Target Compounds							
23)	Chlordane-1	4.311	4.963	16402851	267.8E6	465.154	467.019
24)	Chlordane-2	4.812	5.431	19895246	241.2E6	488.490	451.794
25)	Chlordane-3	5.381	6.077	55884274	1021.6E6	471.616	457.130
26)	Chlordane-4	5.439	6.151	47044836	1173.2E6	485.124	454.860
27)	Chlordane-5	6.276	6.955	21138924	229.6E6	484.918	466.775



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050721\
Data File : PD062787.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2021 19:49
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 09:33:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

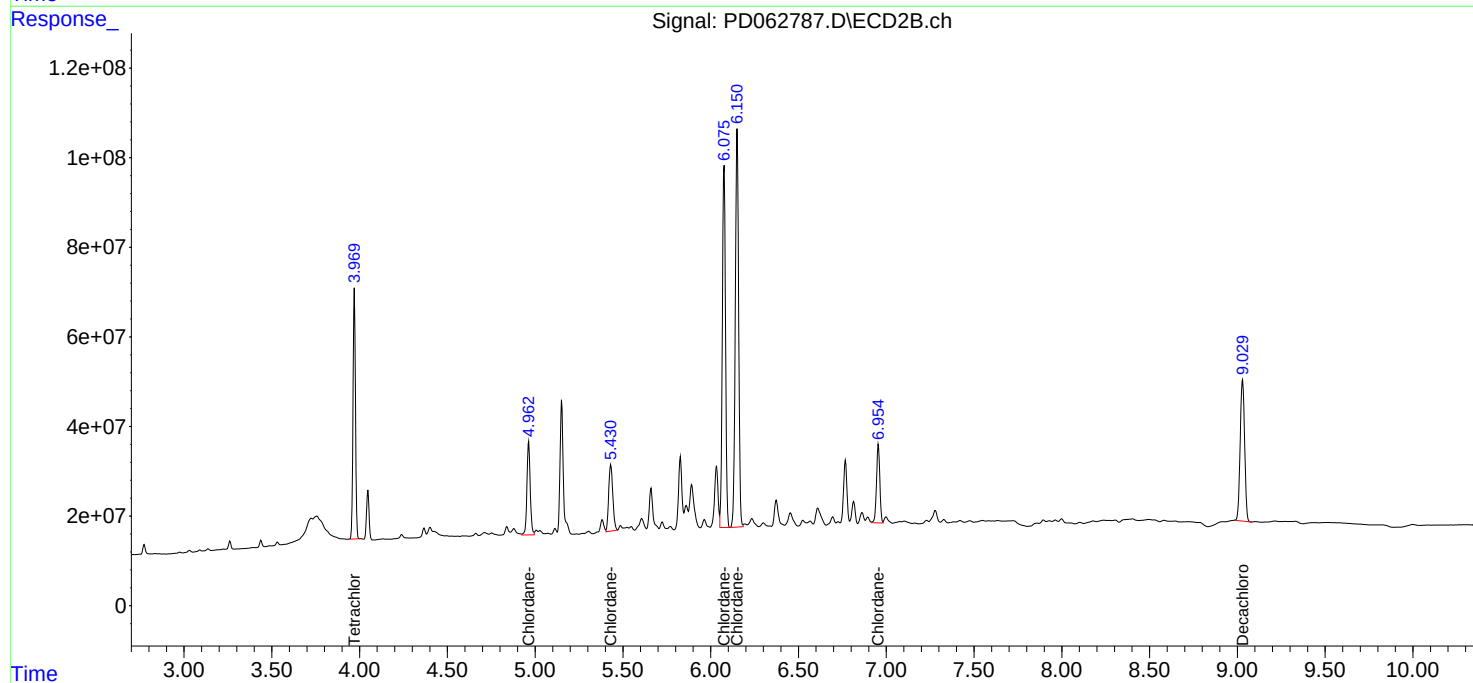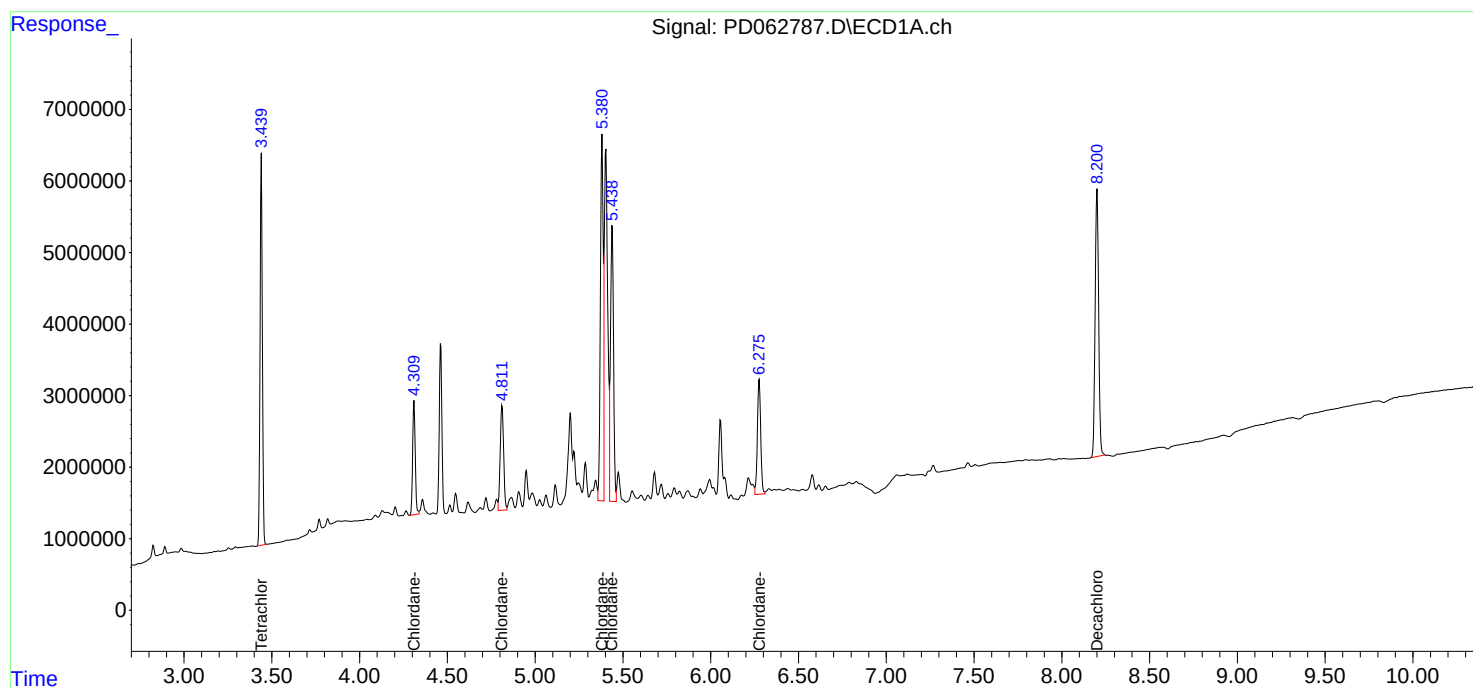


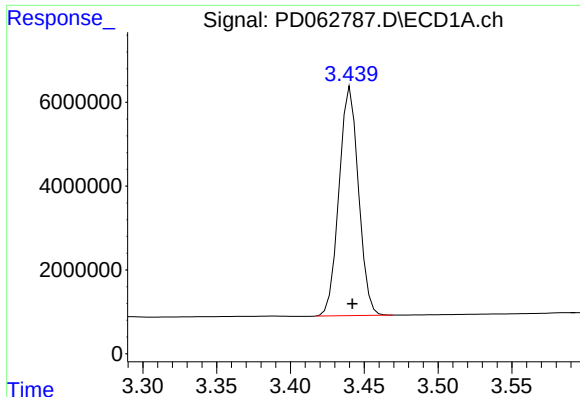

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: -0.001 min
Response: 50123758
Conc: 56.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

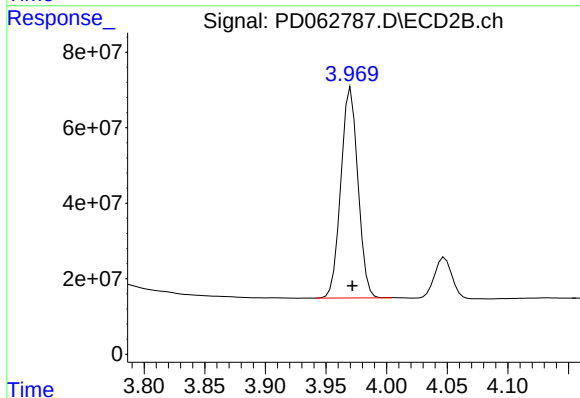


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.001 min
Response: 545669638
Conc: 47.13 ng/ml

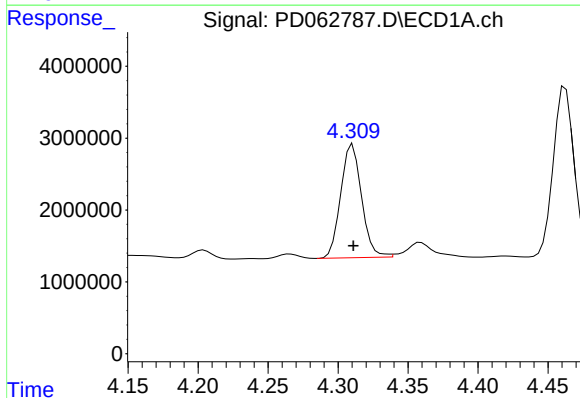


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 16402851
Conc: 465.15 ng/ml

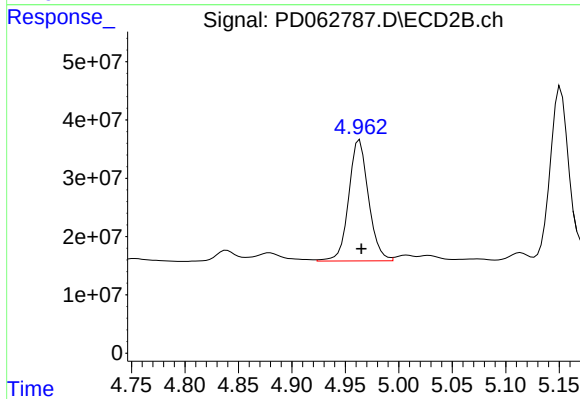

#23 Chlordane-1


R.T.: 4.963 min
Delta R.T.: -0.002 min
Response: 267800041
Conc: 467.02 ng/ml

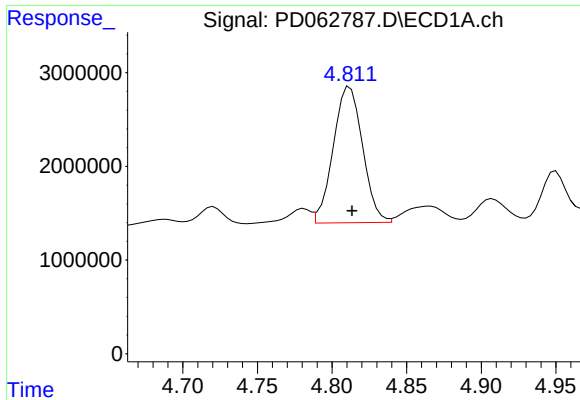

#24 Chlordane-2


R.T.: 4.812 min
Delta R.T.: -0.001 min
Response: 19895246
Conc: 488.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

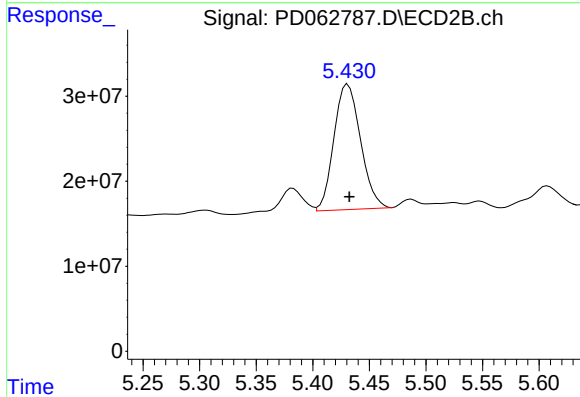


#24 Chlordane-2

R.T.: 5.431 min
Delta R.T.: -0.002 min
Response: 241198811
Conc: 451.79 ng/ml

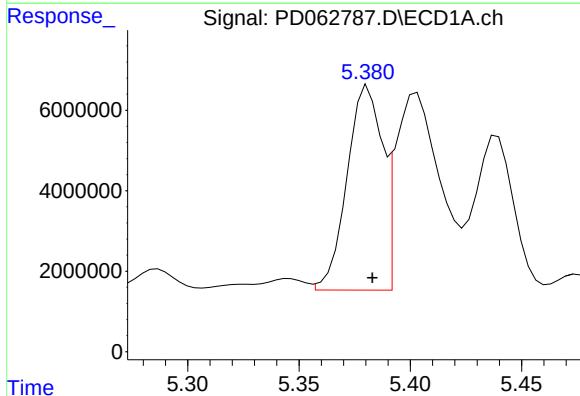


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: -0.002 min
Response: 55884274
Conc: 471.62 ng/ml

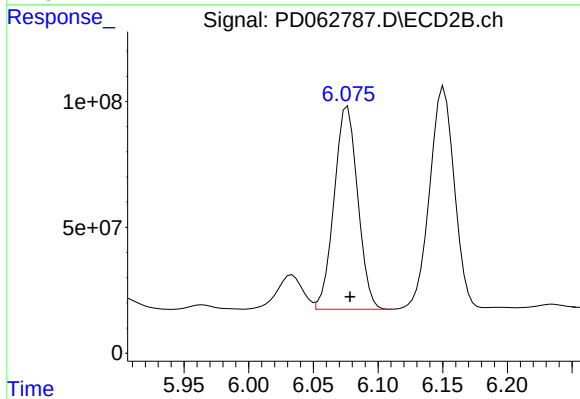

#25 Chlordane-3


R.T.: 6.077 min
Delta R.T.: -0.002 min
Response: 1021644517
Conc: 457.13 ng/ml

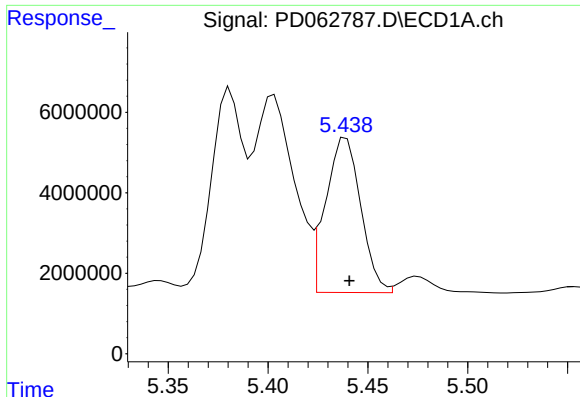

#26 Chlordane-4


R.T.: 5.439 min
Delta R.T.: -0.002 min
Response: 47044836
Conc: 485.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

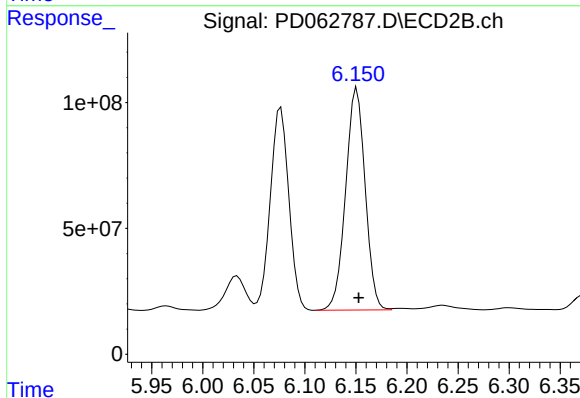


#26 Chlordane-4

R.T.: 6.151 min
Delta R.T.: -0.002 min
Response: 1173216509
Conc: 454.86 ng/ml

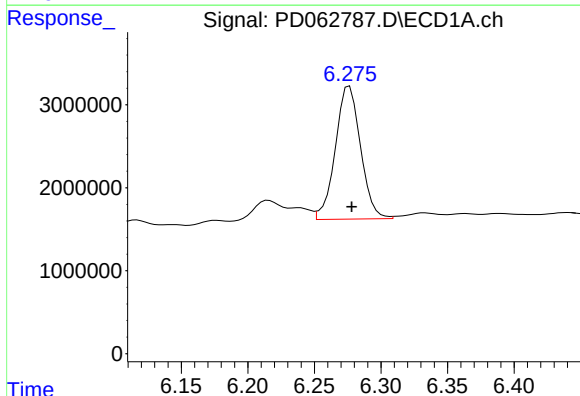


#27 Chlordane-5

R.T.: 6.276 min
Delta R.T.: -0.002 min
Response: 21138924
Conc: 484.92 ng/ml

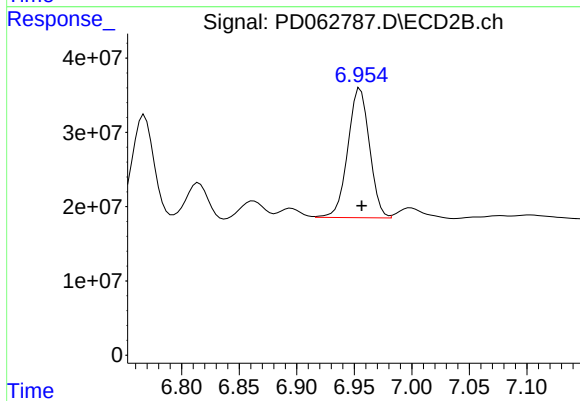

#27 Chlordane-5


R.T.: 6.955 min
Delta R.T.: -0.001 min
Response: 229580666
Conc: 466.78 ng/ml

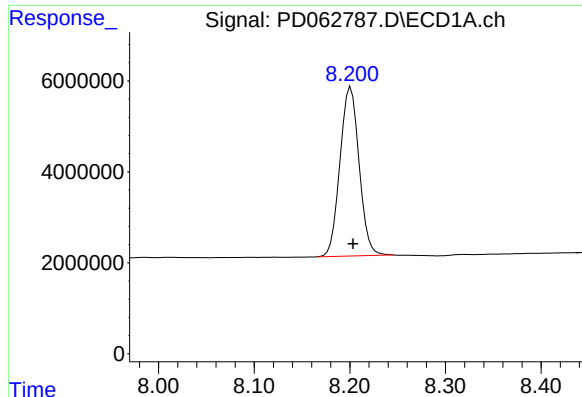

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: -0.002 min
Response: 51760069
Conc: 48.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

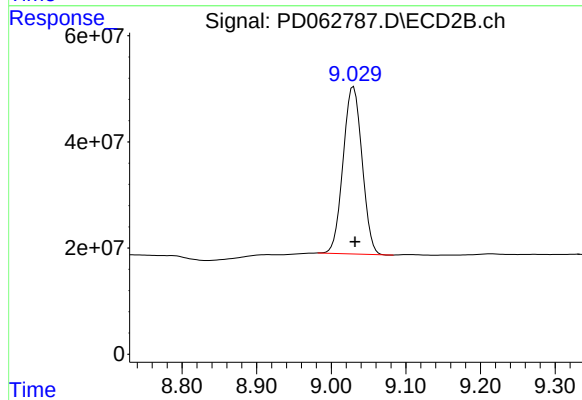

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.002 min
Response: 555448661
Conc: 48.14 ng/ml