

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050722\
 Data File : PD069458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2022 18:29
 Operator : AR\AJ
 Sample : RESC025
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC027

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 00:03:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 18 23:46:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.175	23124768	233.7E6	19.023	18.426
2)	SA Decachlor...	8.201	9.371	46754243	283.1E6	37.694	38.761
Target Compounds							
2)	A alpha-BHC	3.884	4.571	15722500	158.4E6	9.217	8.672
3)	MA gamma-BHC...	4.168	4.862	15685786	153.1E6	9.368	9.405
4)	MA Heptachlor	4.465	5.389	15111210	146.5E6	9.340	9.257
5)	MB Aldrin	4.712	5.701	15315146	152.6E6	10.437	10.634
6)	B beta-BHC	4.418	5.025	7840729	70772117	10.992	10.386
7)	B delta-BHC	4.622	5.251	15405641	81351355	10.207	7.180 #
8)	B Heptachlo...	5.156	6.090	14444306	77543885	10.400	7.191 #
9)	A Endosulfan I	5.495	6.452	12835121	111.6E6	9.332	8.835
10)	B trans-Chl...	5.382	6.327	14846172	132.4E6	10.448	10.087
11)	B cis-Chlor...	5.441	6.401	14396692	125.2E6	10.334	9.820
12)	B 4,4'-DDE	5.607	6.551	26449850	239.0E6	20.315	20.685
13)	MA Dieldrin	5.738	6.711	27309610	235.7E6	18.417	18.517
14)	MA Endrin	5.997	6.931	24229133	186.0E6	18.608	18.389
15)	B Endosulfa...	6.271	7.136	24025631	195.1E6	20.603	20.388
16)	A 4,4'-DDD	6.124	7.042	21332345	178.8E6	18.202	18.071
17)	MA 4,4'-DDT	6.364	7.345	20993693	179.6E6	17.953	18.773
18)	B Endrin al...	6.441	7.260	22074045	172.8E6	21.233	20.924
19)	B Endosulfa...	6.653	7.485	25361975	197.7E6	20.695	21.136
20)	A Methoxychlor	6.915	7.798	62985425	431.4E6	95.879	97.868
21)	B Endrin ke...	7.146	7.960	30026849	205.7E6	22.044	21.508

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050722\
Data File : PD069458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2022 18:29
Operator : AR\AJ
Sample : RESC025
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 00:03:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 18 23:46:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

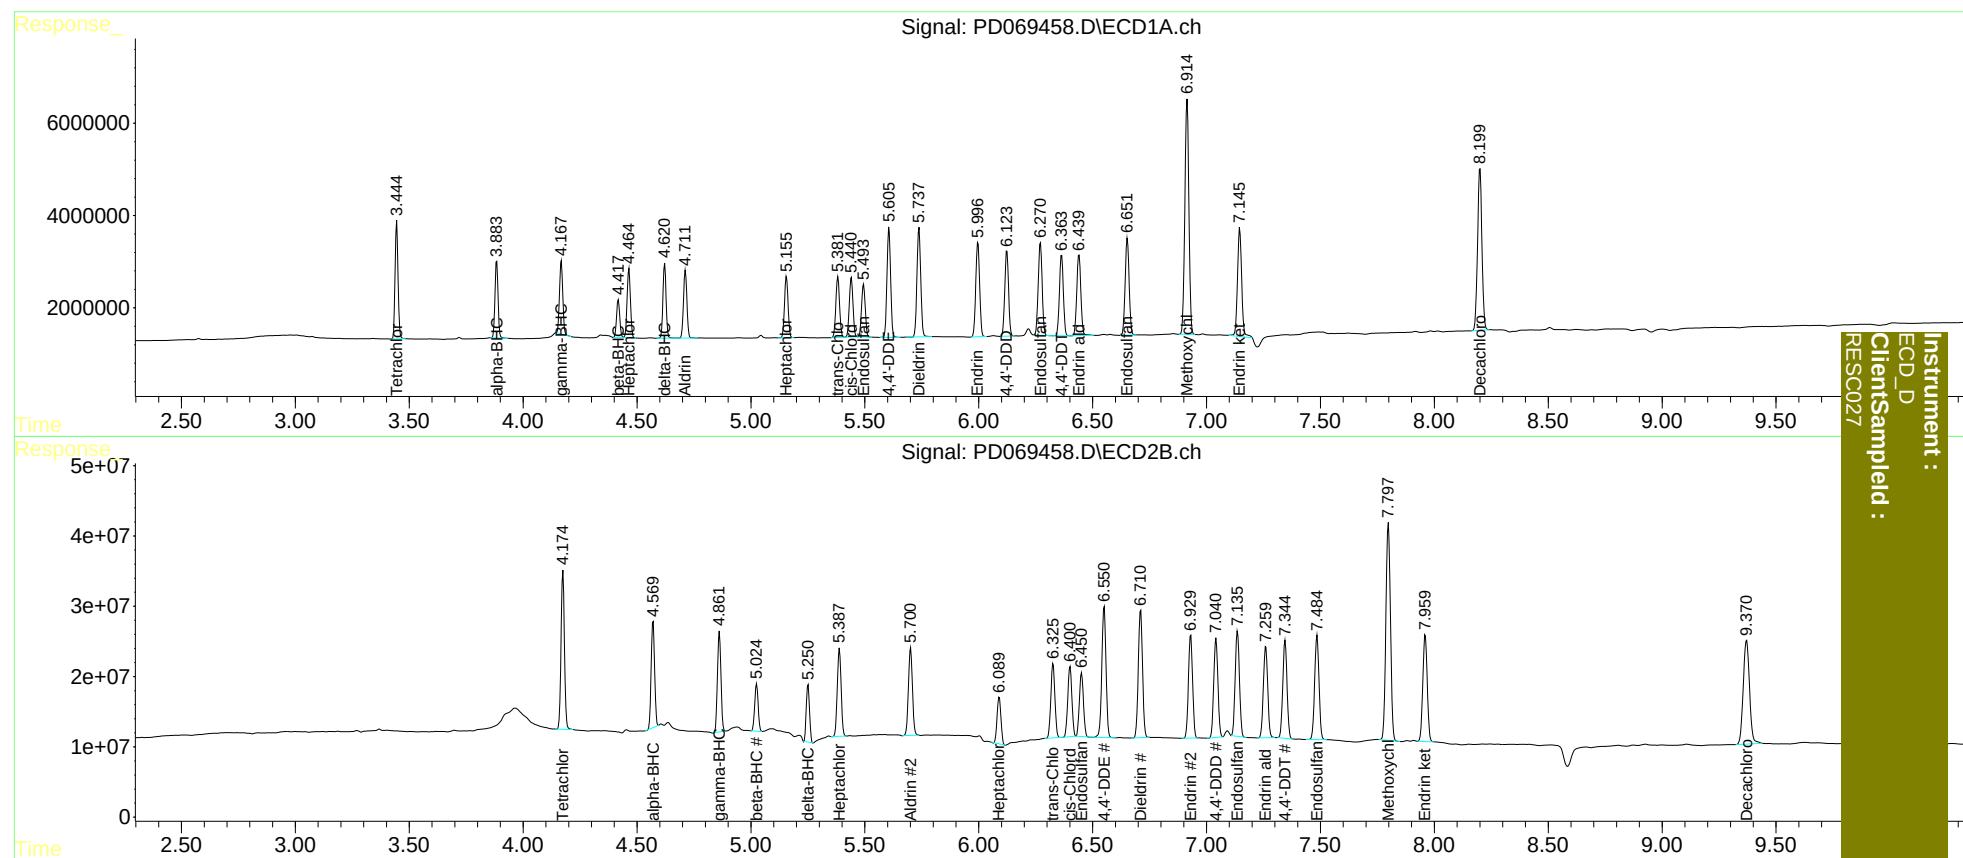

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050722\
Data File : PD069458.D
Acq On : 06 May 2022 18:29
Operator : AR\AJ
Sample : RESC025
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC027

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050722CLP.M
Title : GC Extractables
Last Update : Wed May 18 23:46:25 2022
Integrator: ChemStation

RT#1	RT#2	Resolution
3.445	3.884	100.00%
3.884	4.168	100.00%
4.168	4.418	100.00%
4.418	4.465	100.00%
4.465	4.622	100.00%
4.622	4.712	100.00%
4.712	5.156	100.00%
5.156	5.382	100.00%
5.382	5.441	100.00%
5.441	5.495	100.00%
5.495	5.607	100.00%
5.607	5.738	100.00%
5.738	5.997	100.00%
5.997	6.124	100.00%
6.124	6.271	100.00%
6.271	6.364	100.00%
6.364	6.441	100.00%
6.441	6.653	100.00%
6.653	6.915	100.00%
6.915	7.146	100.00%
7.146	8.201	100.00%

Signal #2

4.175	4.571	100.00%
4.571	4.862	100.00%
4.862	5.025	100.00%
5.025	5.251	100.00%
5.251	5.389	100.00%
5.389	5.701	100.00%
5.701	6.090	100.00%
6.090	6.327	100.00%
6.327	6.401	100.00%
6.401	6.452	100.00%
6.452	6.551	100.00%
6.551	6.711	100.00%
6.711	6.931	100.00%
6.931	7.042	100.00%
7.042	7.136	100.00%
7.136	7.260	100.00%
7.260	7.345	100.00%
7.345	7.485	100.00%
7.485	7.798	100.00%
7.798	7.960	100.00%
7.960	9.371	100.00%