

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 08:52
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 07:56:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	3.873	0.000	271035	0	0.195	N.D.	#
7) B	delta-BHC	0.000	5.028	0	11523450	N.D.	0.638	#
8) B	Heptachlo...	0.000	5.837	0	156.2E6	N.D.	9.778	#
9) A	Endosulfan I	0.000	6.184f	0	5651096	N.D.	0.383	#
11) B	alpha-Chl...	0.000	6.134f	0	4951887	N.D.	0.324	#
14) MA	Endrin	6.001	6.670	1385693	62397767	1.247	4.438	#
18) B	Endrin al...	6.468f	0.000	3304658	0	3.542	N.D.	#
26)	Chlordane-4	0.000	6.134f	0	4951887	N.D.	1.920	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 08:52
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 07:56:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

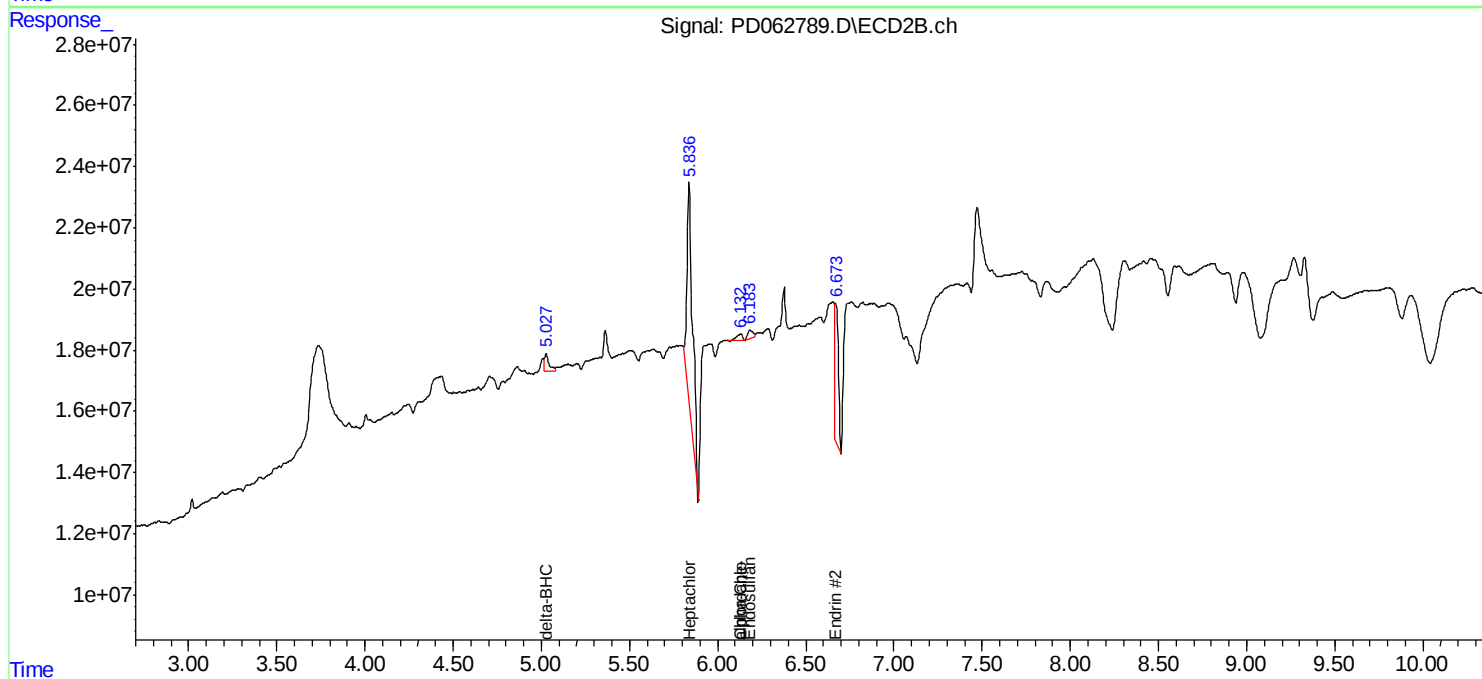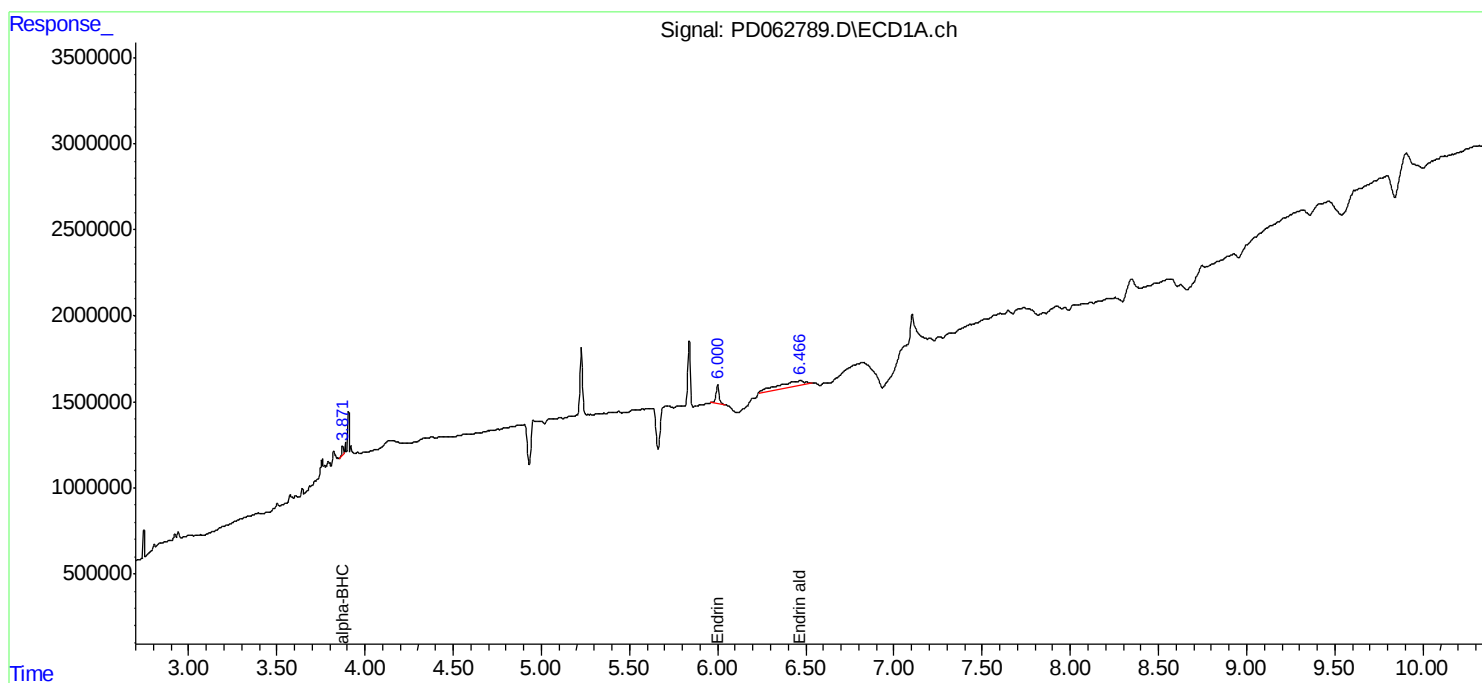


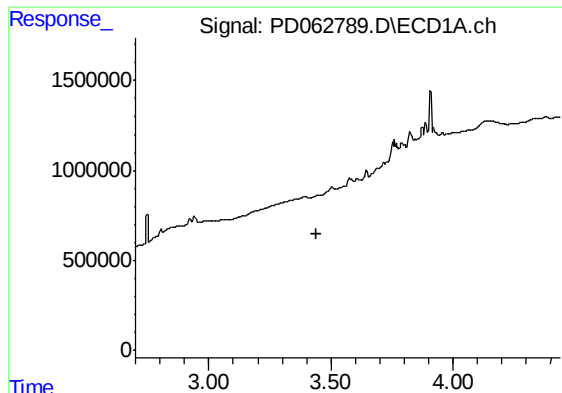

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

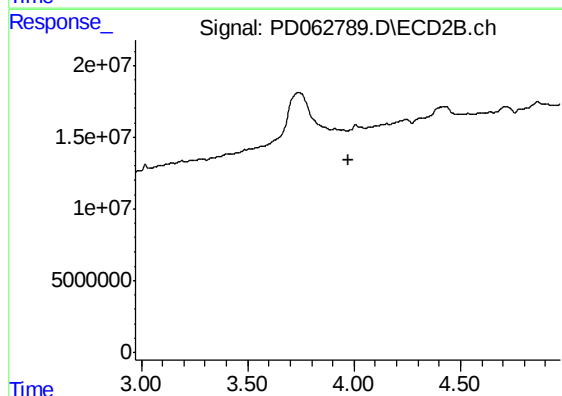


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.972 min
Response: 0
Conc: N.D.

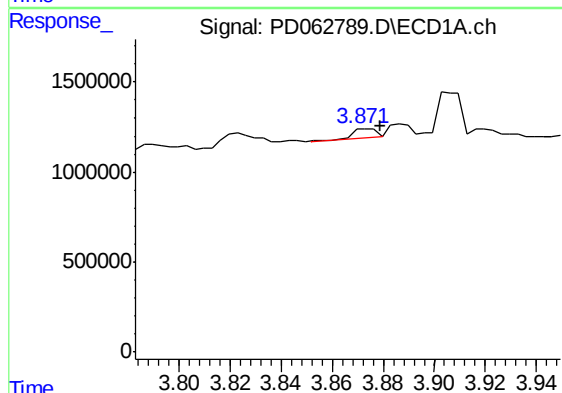


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: -0.006 min
Response: 271035
Conc: 0.19 ng/ml

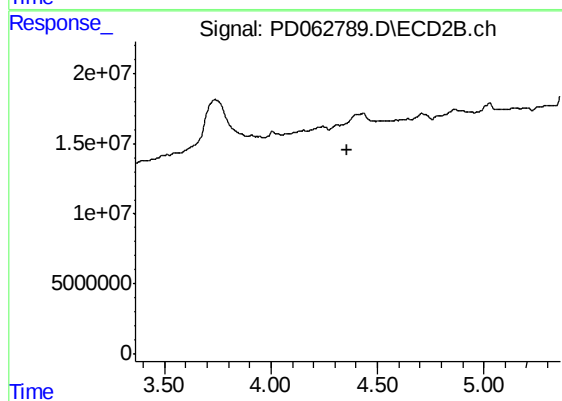

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.360 min
Response: 0
Conc: N.D.

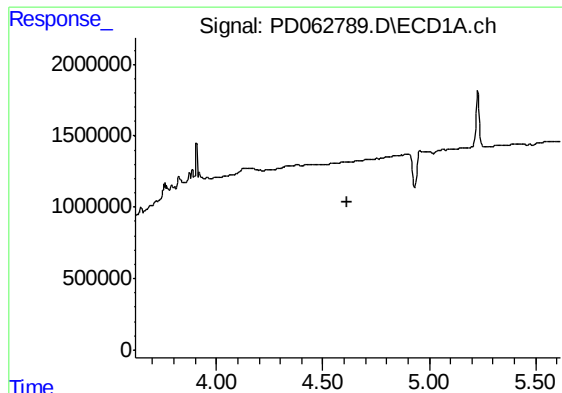

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

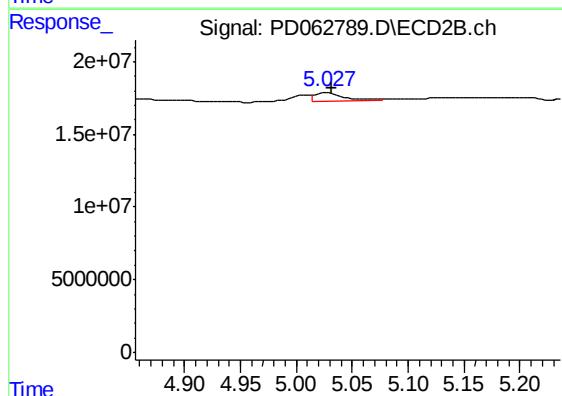


#7 delta-BHC

R.T.: 5.028 min
Delta R.T.: -0.003 min
Response: 11523450
Conc: 0.64 ng/ml

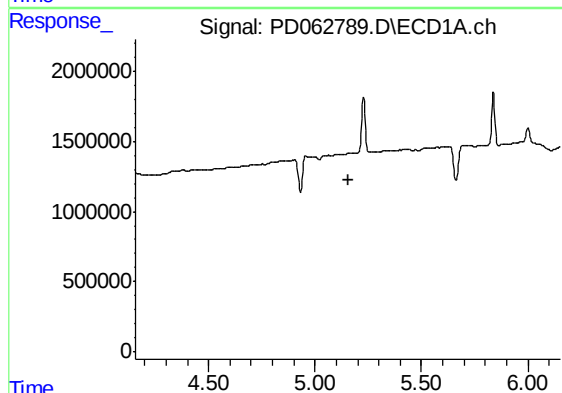


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.155 min
Response: 0
Conc: N.D.

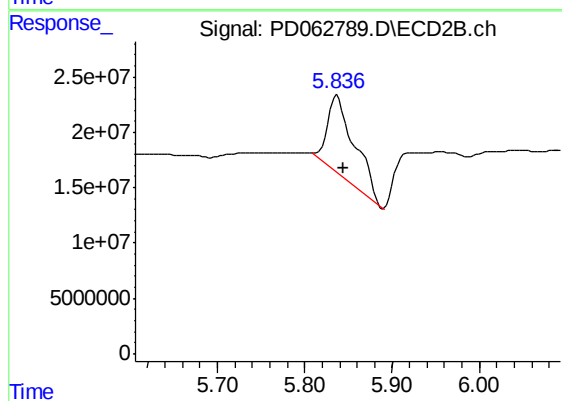

#8 Heptachlor epoxide


R.T.: 5.837 min
Delta R.T.: -0.008 min
Response: 156198709
Conc: 9.78 ng/ml

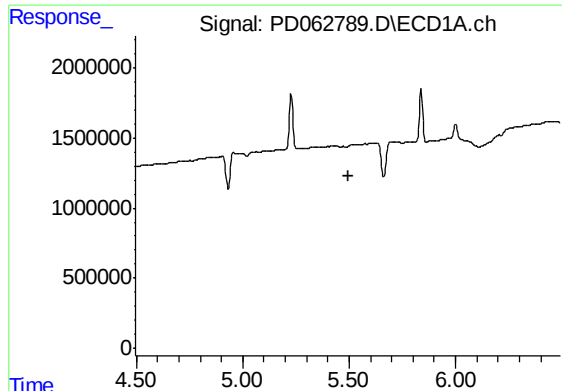

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

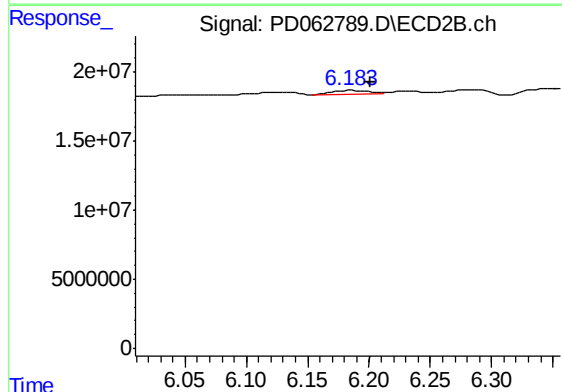


#9 Endosulfan I

R.T.: 6.184 min
Delta R.T.: -0.016 min
Response: 5651096
Conc: 0.38 ng/ml

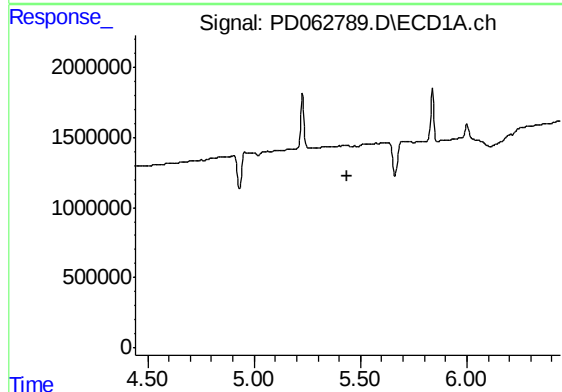


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.441 min
Response: 0
Conc: N.D.

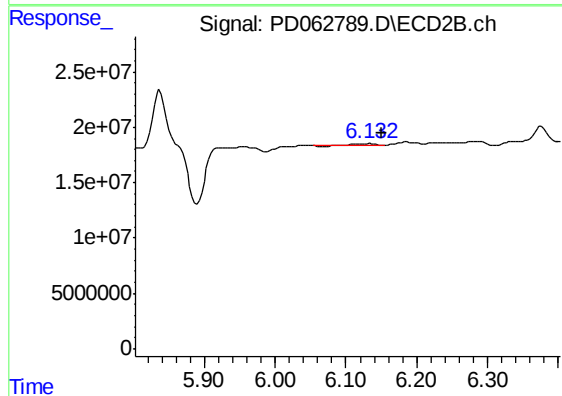

#11 alpha-Chlordane


R.T.: 6.134 min
Delta R.T.: -0.017 min
Response: 4951887
Conc: 0.32 ng/ml

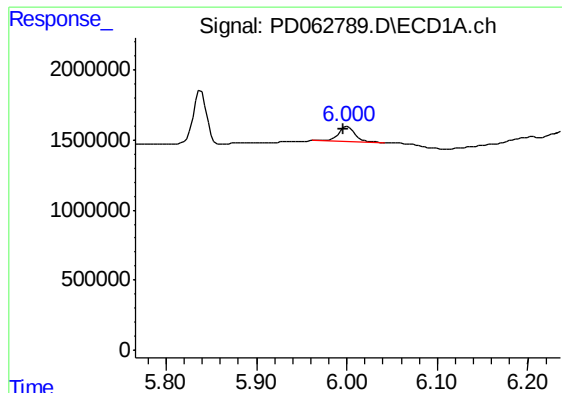

#14 Endrin


R.T.: 6.001 min
Delta R.T.: 0.005 min
Response: 1385693
Conc: 1.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

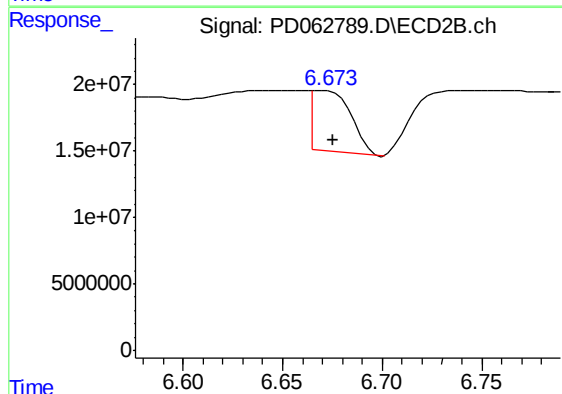


#14 Endrin

R.T.: 6.670 min
Delta R.T.: -0.005 min
Response: 62397767
Conc: 4.44 ng/ml

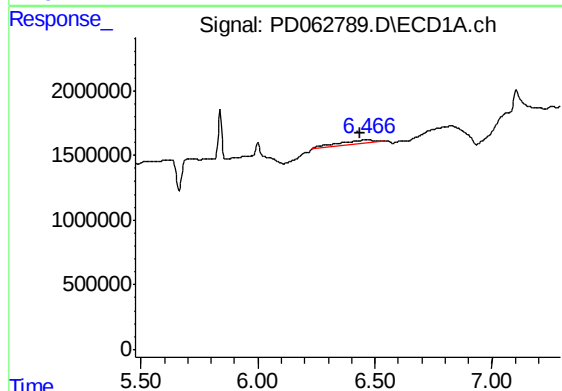


#18 Endrin aldehyde

R.T.: 6.468 min
Delta R.T.: 0.030 min
Response: 3304658
Conc: 3.54 ng/ml

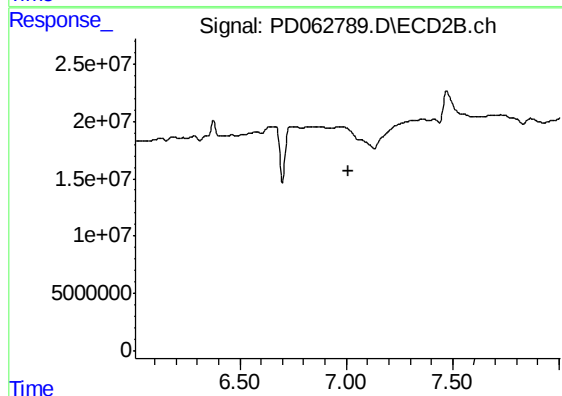

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.009 min
Response: 0
Conc: N.D.

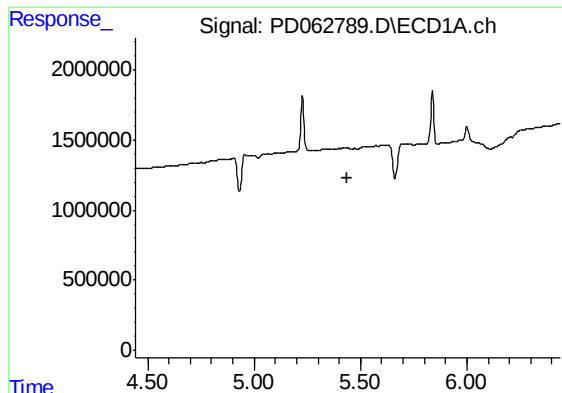

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

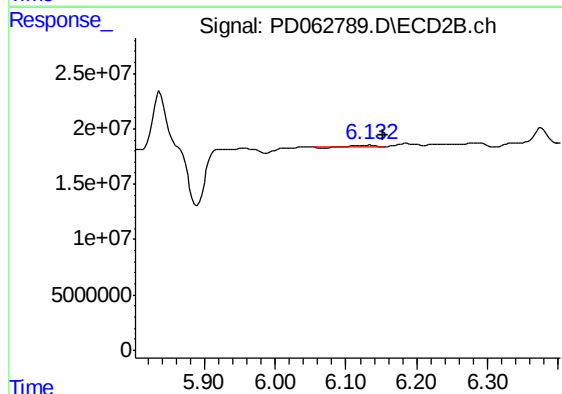


#26 Chlordane-4

R.T.: 6.134 min
Delta R.T.: -0.019 min
Response: 4951887
Conc: 1.92 ng/ml

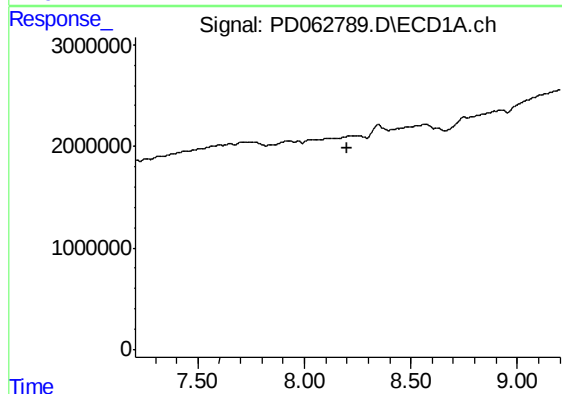

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.203 min
Response: 0
Conc: N.D.

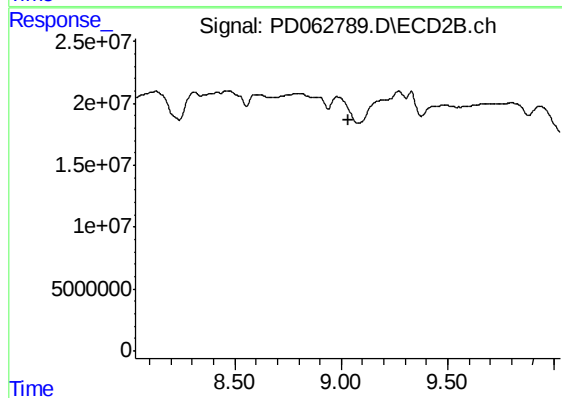

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.032 min
Response: 0
Conc: N.D.