

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
 Data File : PD062819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 18:32
 Operator : AR\AJ
 Sample : M2295-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DRUM-D-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 08:02:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	19444648	242.4E6	21.867	20.939
28)	SA Decachlor...	8.201	9.031	22074991	245.1E6	20.851	21.245
Target Compounds							
5)	MB Aldrin	0.000	5.471	0	1251982	N.D.	0.075 #
6)	B beta-BHC	0.000	4.844f	0	7022223	N.D.	0.921 #
7)	B delta-BHC	0.000	5.009f	0	38936811	N.D.	2.157 #
8)	B Heptachlo...	0.000	5.854	0	12339671	N.D.	0.772 #
15)	B Endosulfa...	0.000	6.885	0	11938957	N.D.	0.894 #
17)	MA 4,4'-DDT	0.000	7.112	0	15433922	N.D.	1.212 #
23)	Chlordane-1	0.000	4.959	0	1941533	N.D.	3.386 #
24)	Chlordane-2	0.000	5.421	0	4076929	N.D.	7.637 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050821\
Data File : PD062819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 18:32
Operator : AR\AJ
Sample : M2295-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
DRUM-D-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 08:02:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

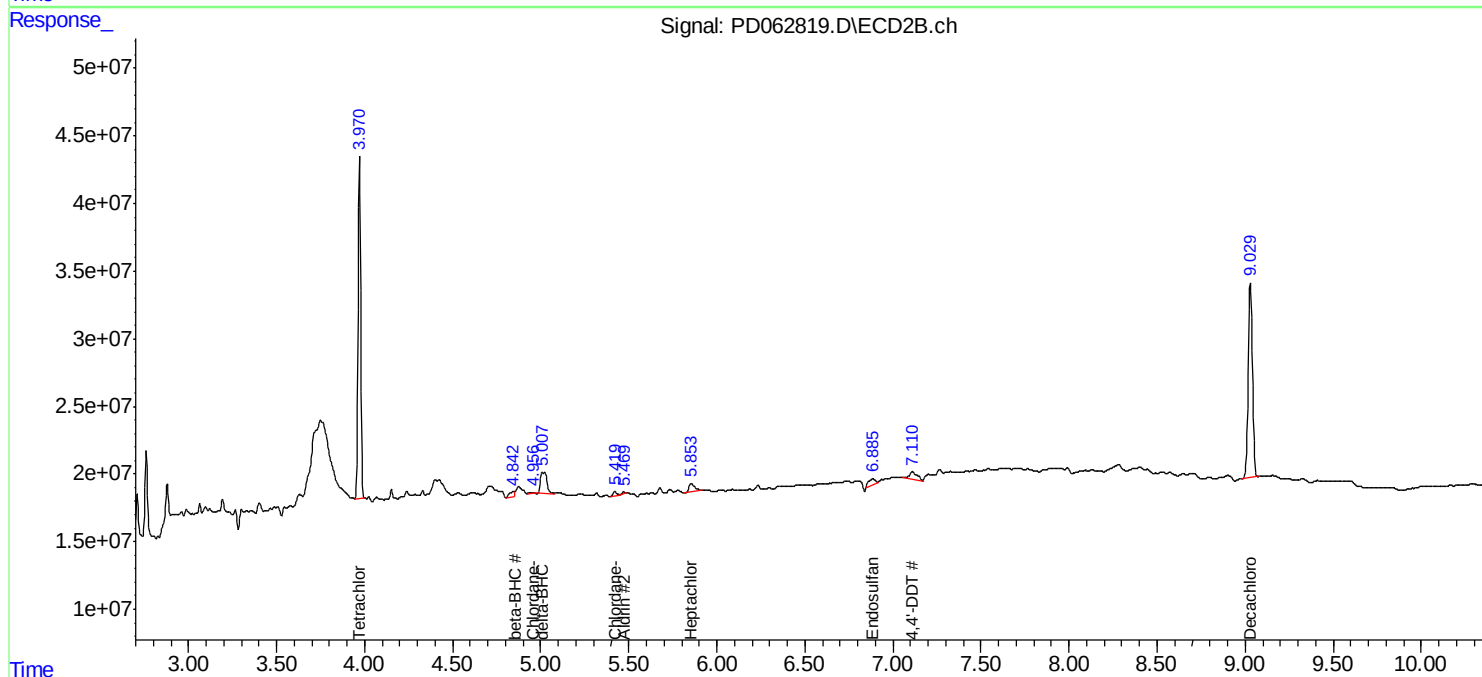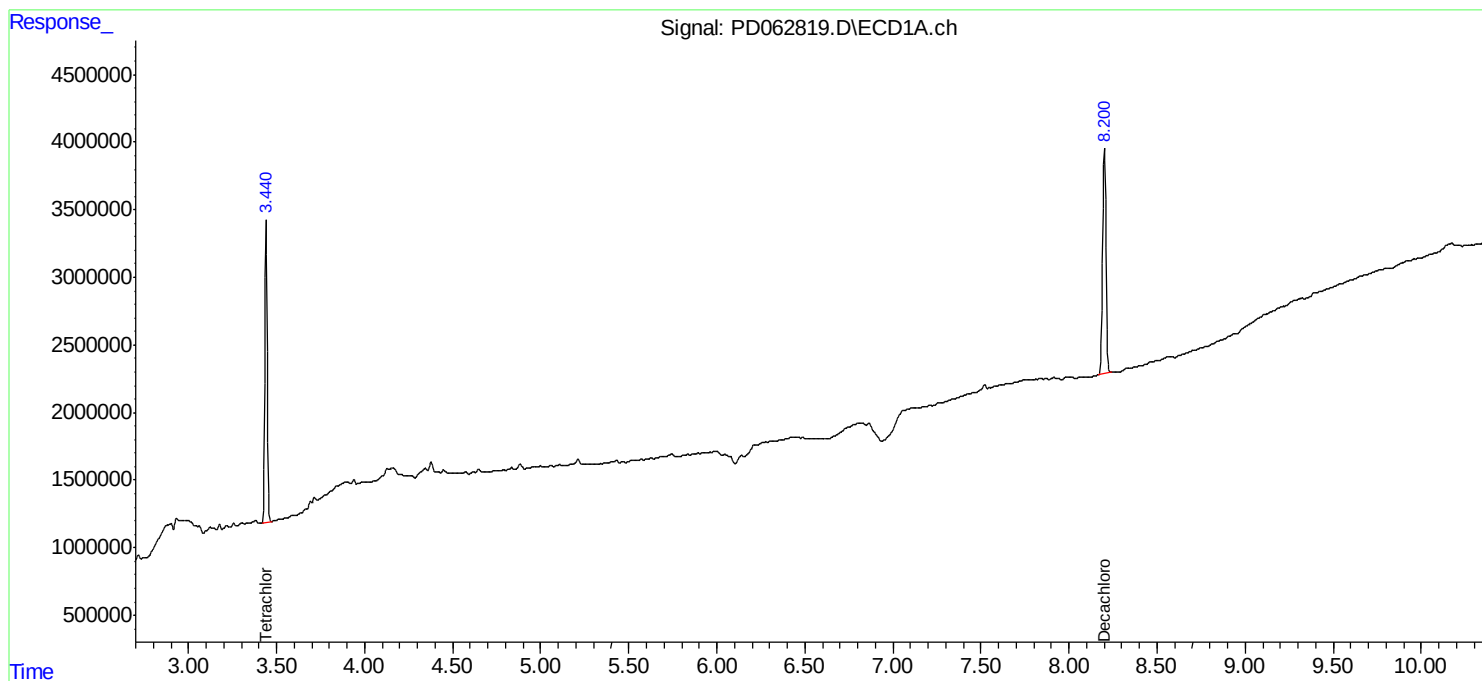


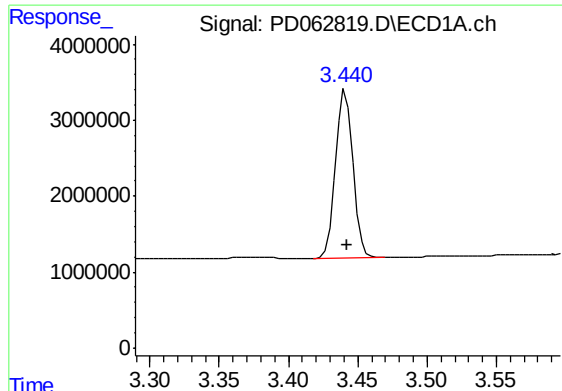

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 19444648
Conc: 21.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
DRUM-D-E

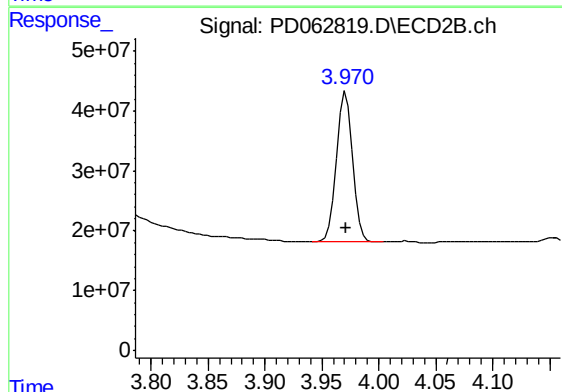


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 242415215
Conc: 20.94 ng/ml

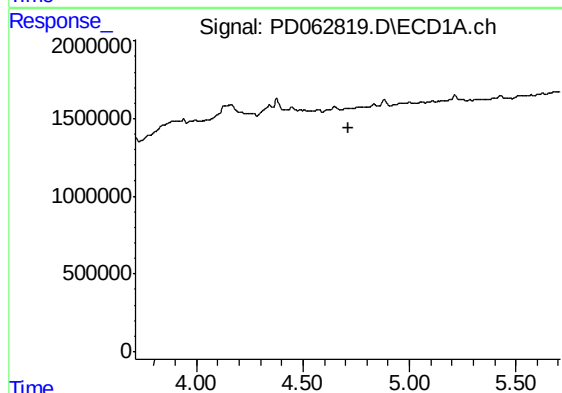


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.712 min
Response: 0
Conc: N.D.

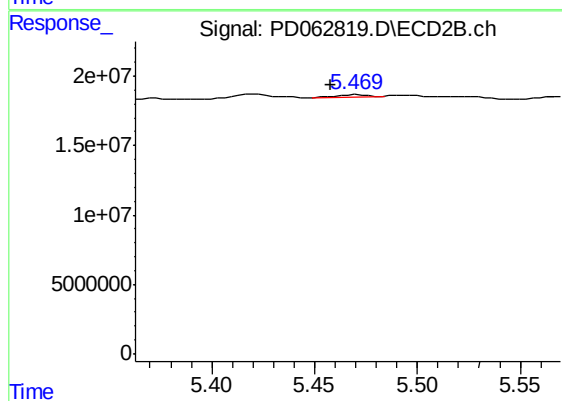

#5 Aldrin


R.T.: 5.471 min
Delta R.T.: 0.013 min
Response: 1251982
Conc: 0.07 ng/ml

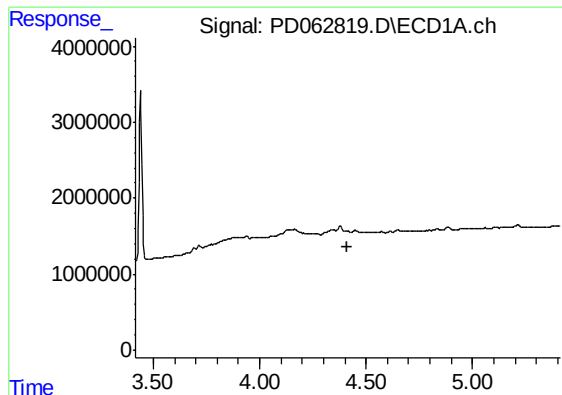

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.413 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DRUM-D-E

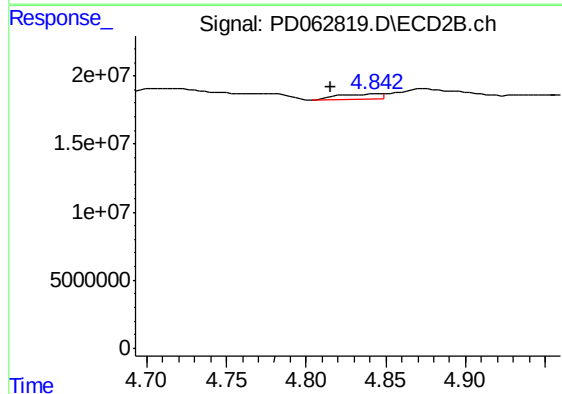


#6 beta-BHC

R.T.: 4.844 min
Delta R.T.: 0.028 min
Response: 7022223
Conc: 0.92 ng/ml

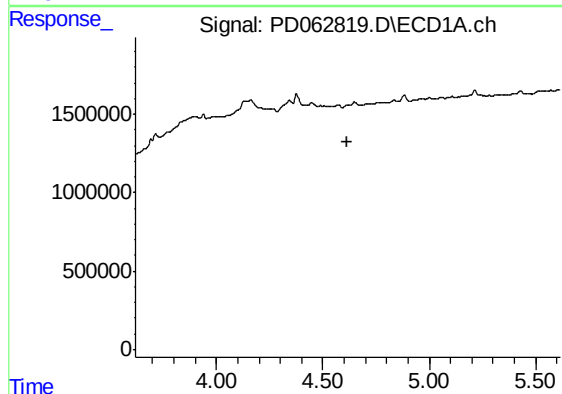


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

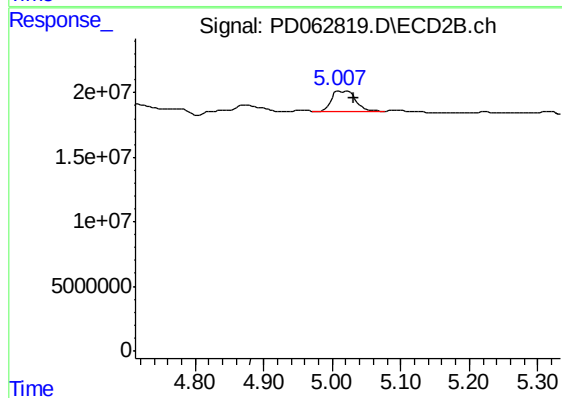

#7 delta-BHC


R.T.: 5.009 min
Delta R.T.: -0.022 min
Response: 38936811
Conc: 2.16 ng/ml

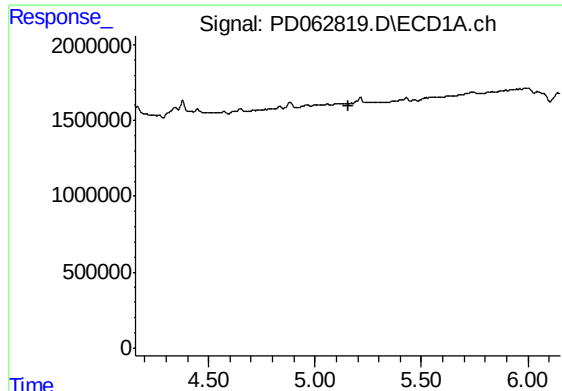

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DRUM-D-E

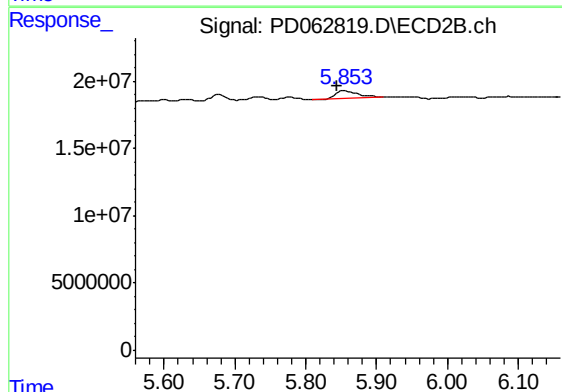


#8 Heptachlor epoxide

R.T.: 5.854 min
Delta R.T.: 0.009 min
Response: 12339671
Conc: 0.77 ng/ml

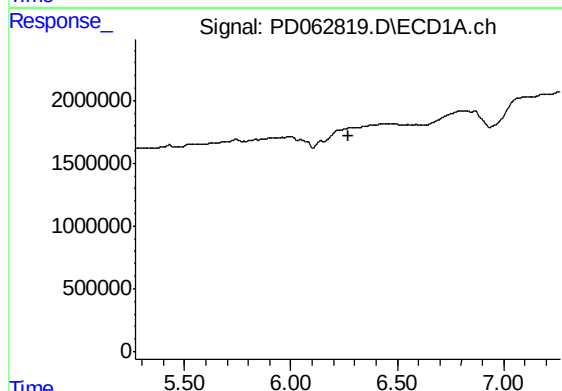


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

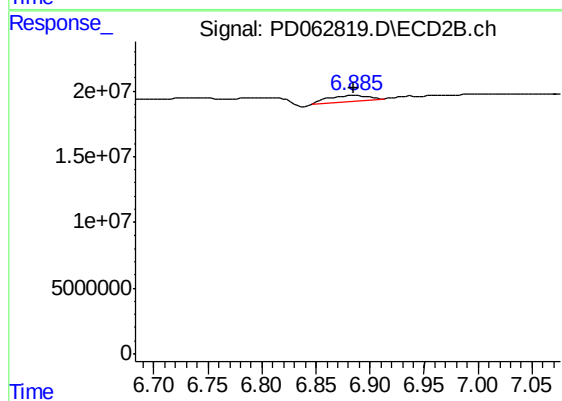

#15 Endosulfan II


R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 11938957
Conc: 0.89 ng/ml

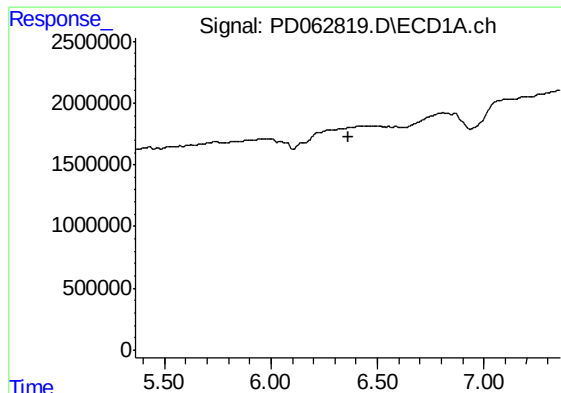

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DRUM-D-E

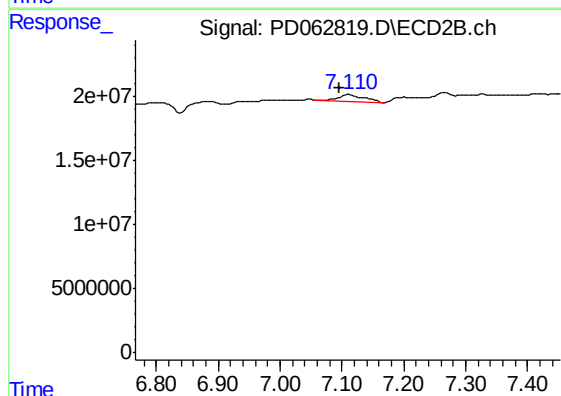


#17 4,4'-DDT

R.T.: 7.112 min
Delta R.T.: 0.015 min
Response: 15433922
Conc: 1.21 ng/ml

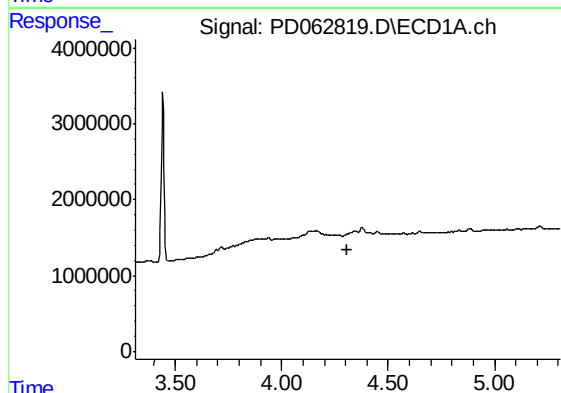


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.311 min
Response: 0
Conc: N.D.

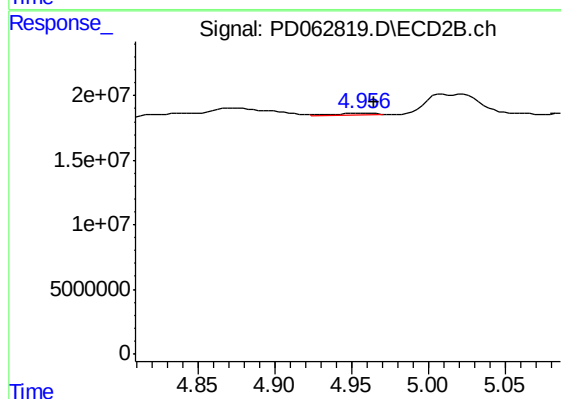

#23 Chlordane-1


R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 1941533
Conc: 3.39 ng/ml

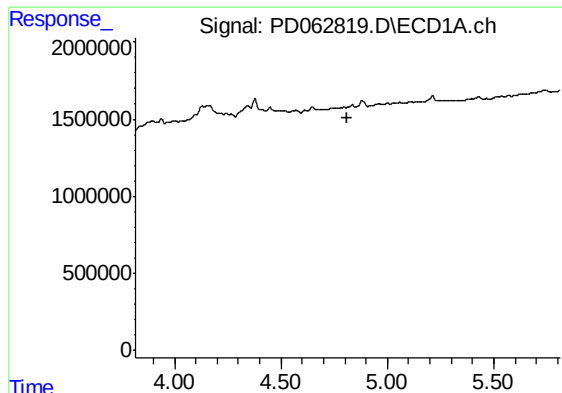

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.813 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DRUM-D-E

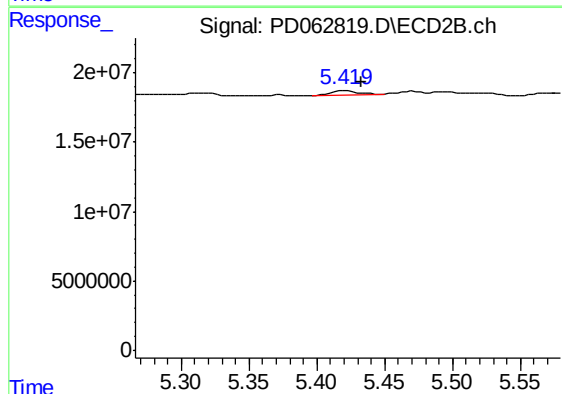


#24 Chlordane-2

R.T.: 5.421 min
Delta R.T.: -0.012 min
Response: 4076929
Conc: 7.64 ng/ml

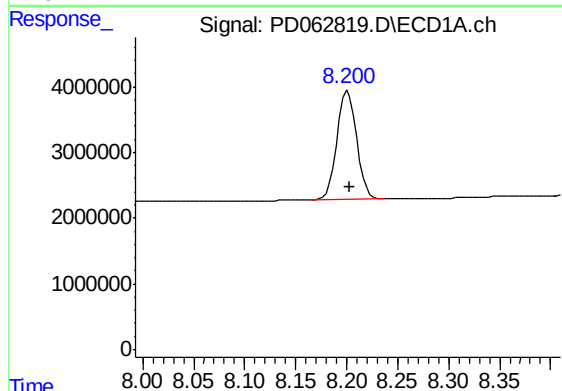

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: -0.002 min
Response: 22074991
Conc: 20.85 ng/ml

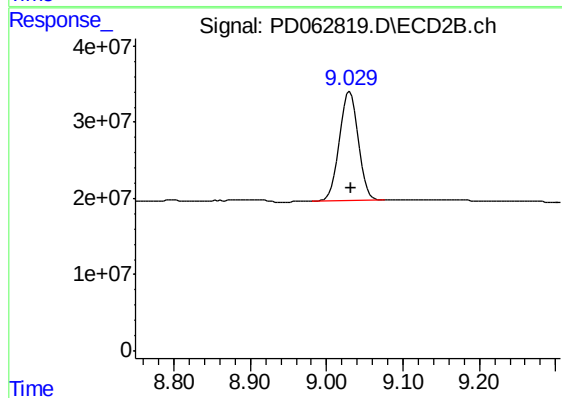

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.002 min
Response: 245143989
Conc: 21.24 ng/ml